


Positive

MS Spectrum

Intensity

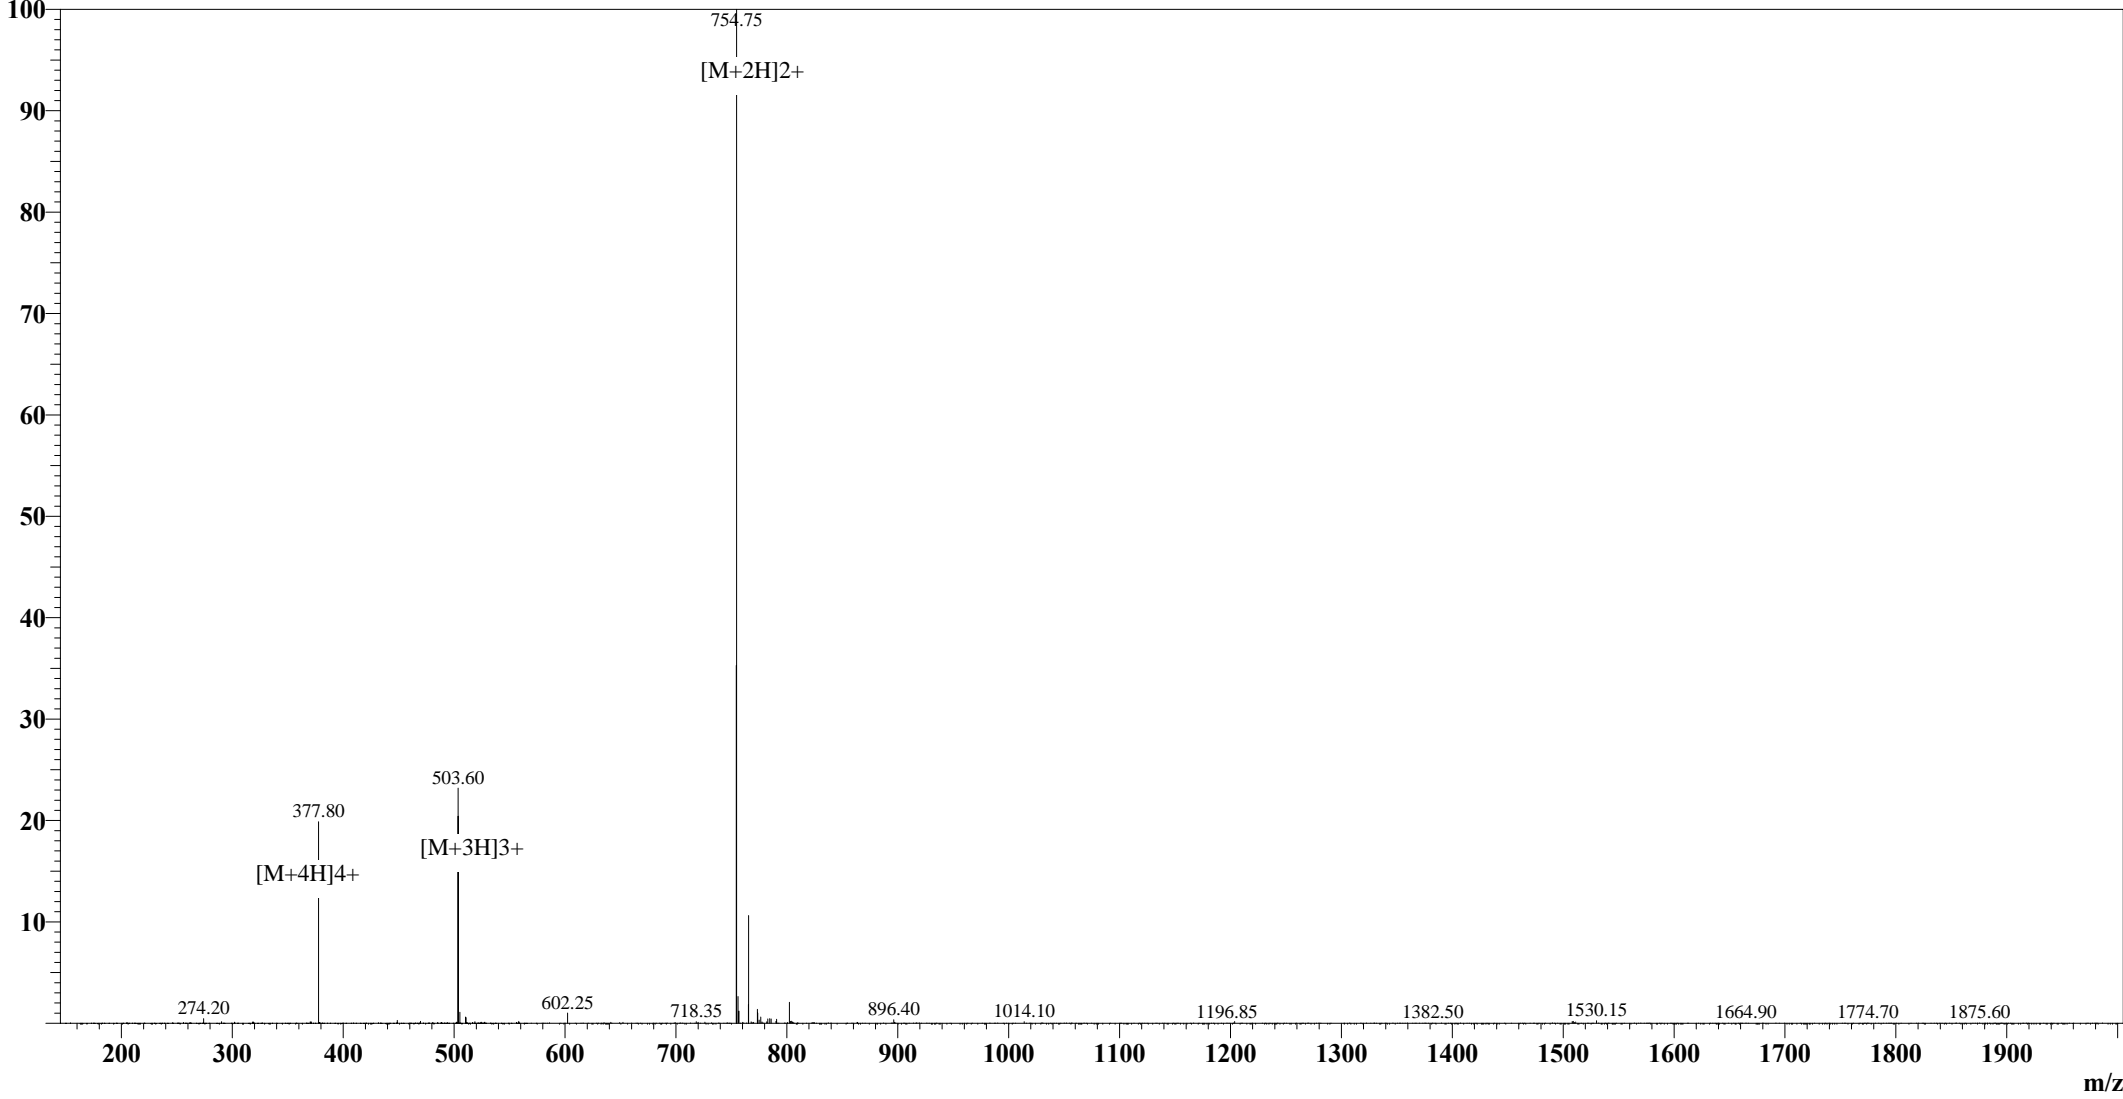

Sample Information

User : Grace  
Date Acquired : 01/20/2010 14:14:20  
Sample Name : Syntide 2  
Cat No. : RP10322  
Lot No. : 87518001011310LQ  
Injection Volum : 1.000µL  
Theoretical MW : 1507.82  
Observed MW : 1507.50

Interface : ESI  
Nebulizing Gas Flow : 4.21 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias : +4.5kv  
Detector : 1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H<sub>2</sub>O/50%MeOH