

Sample Name : Syntide 2
Cat. No. : RP10322
Lot. No. : 87518001011310LQ

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

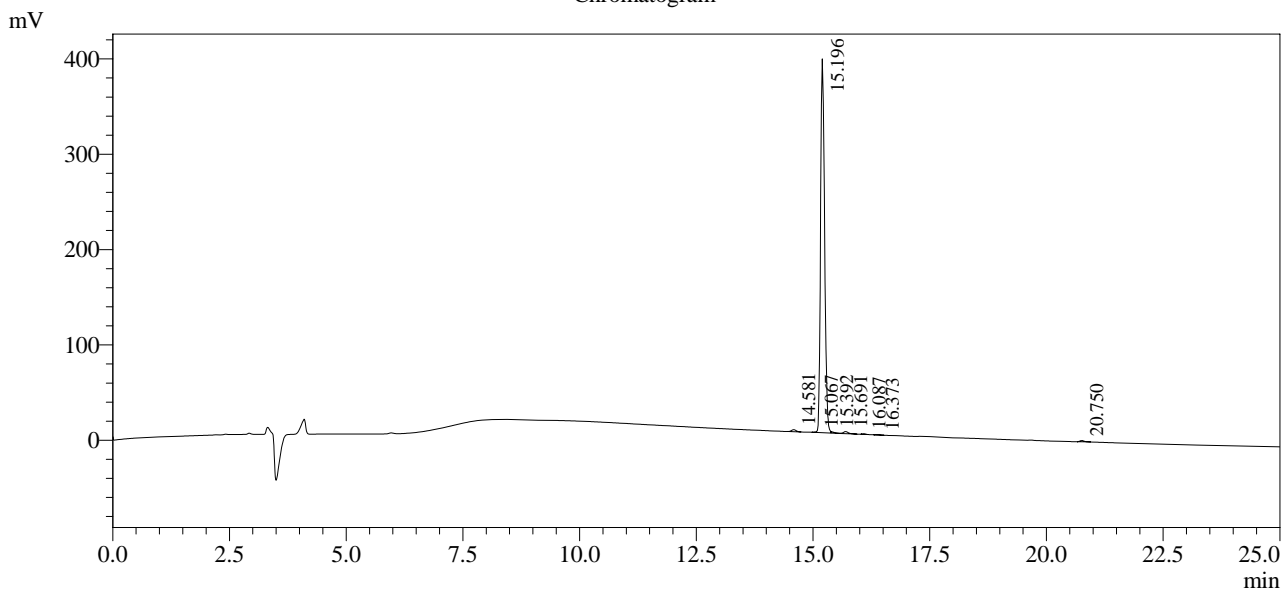

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.581	14233	2102	0.590
2	15.067	2162	732	0.090
3	15.196	2358502	392182	97.801
4	15.392	6626	1518	0.275
5	15.691	17958	2196	0.745
6	16.087	1932	420	0.080
7	16.373	1610	287	0.067
8	20.750	8506	1321	0.353
Total		2411529	400758	100.000