

Sample Name :LL37 (Human)
 Cat. No. :RP13323
 Lot. No. :85691003121409BF

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

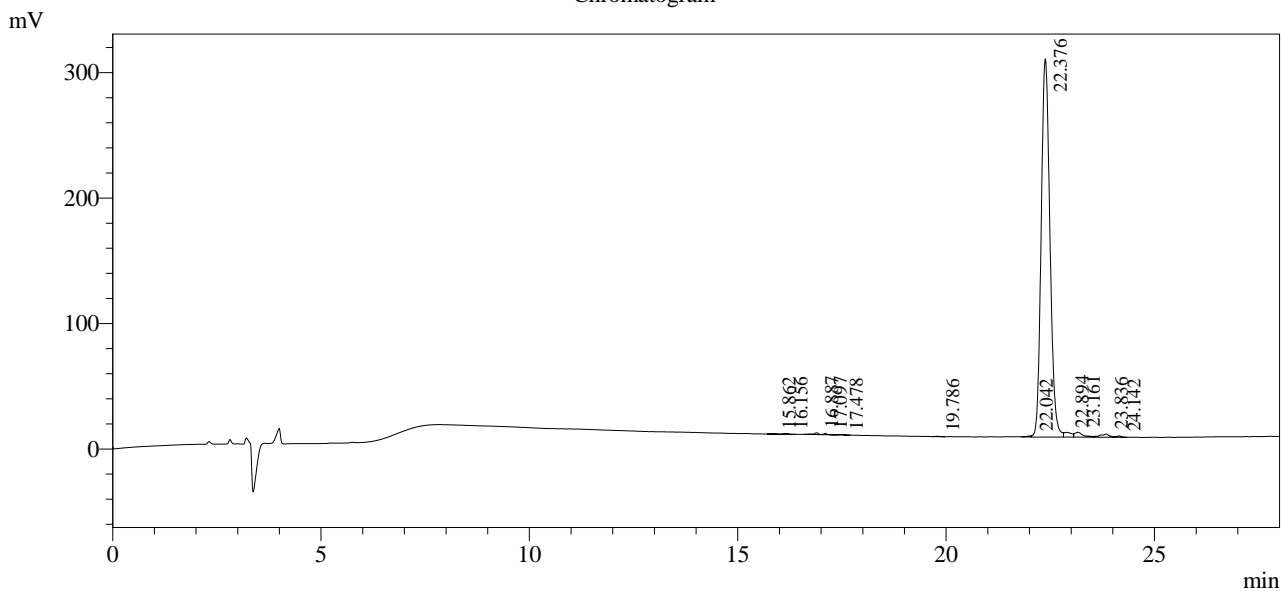

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.862	1722	259	0.038
2	16.156	4600	622	0.100
3	16.887	12018	1449	0.262
4	17.097	6117	1059	0.133
5	17.478	3857	405	0.084
6	19.786	1845	296	0.040
7	22.042	7468	981	0.163
8	22.376	4401131	301454	95.994
9	22.894	47156	3781	1.029
10	23.161	54062	3836	1.179
11	23.836	37900	2549	0.827
12	24.142	6918	1077	0.151
Total		4584793	317769	100.000