


Positive

MS Spectrum

Intensity

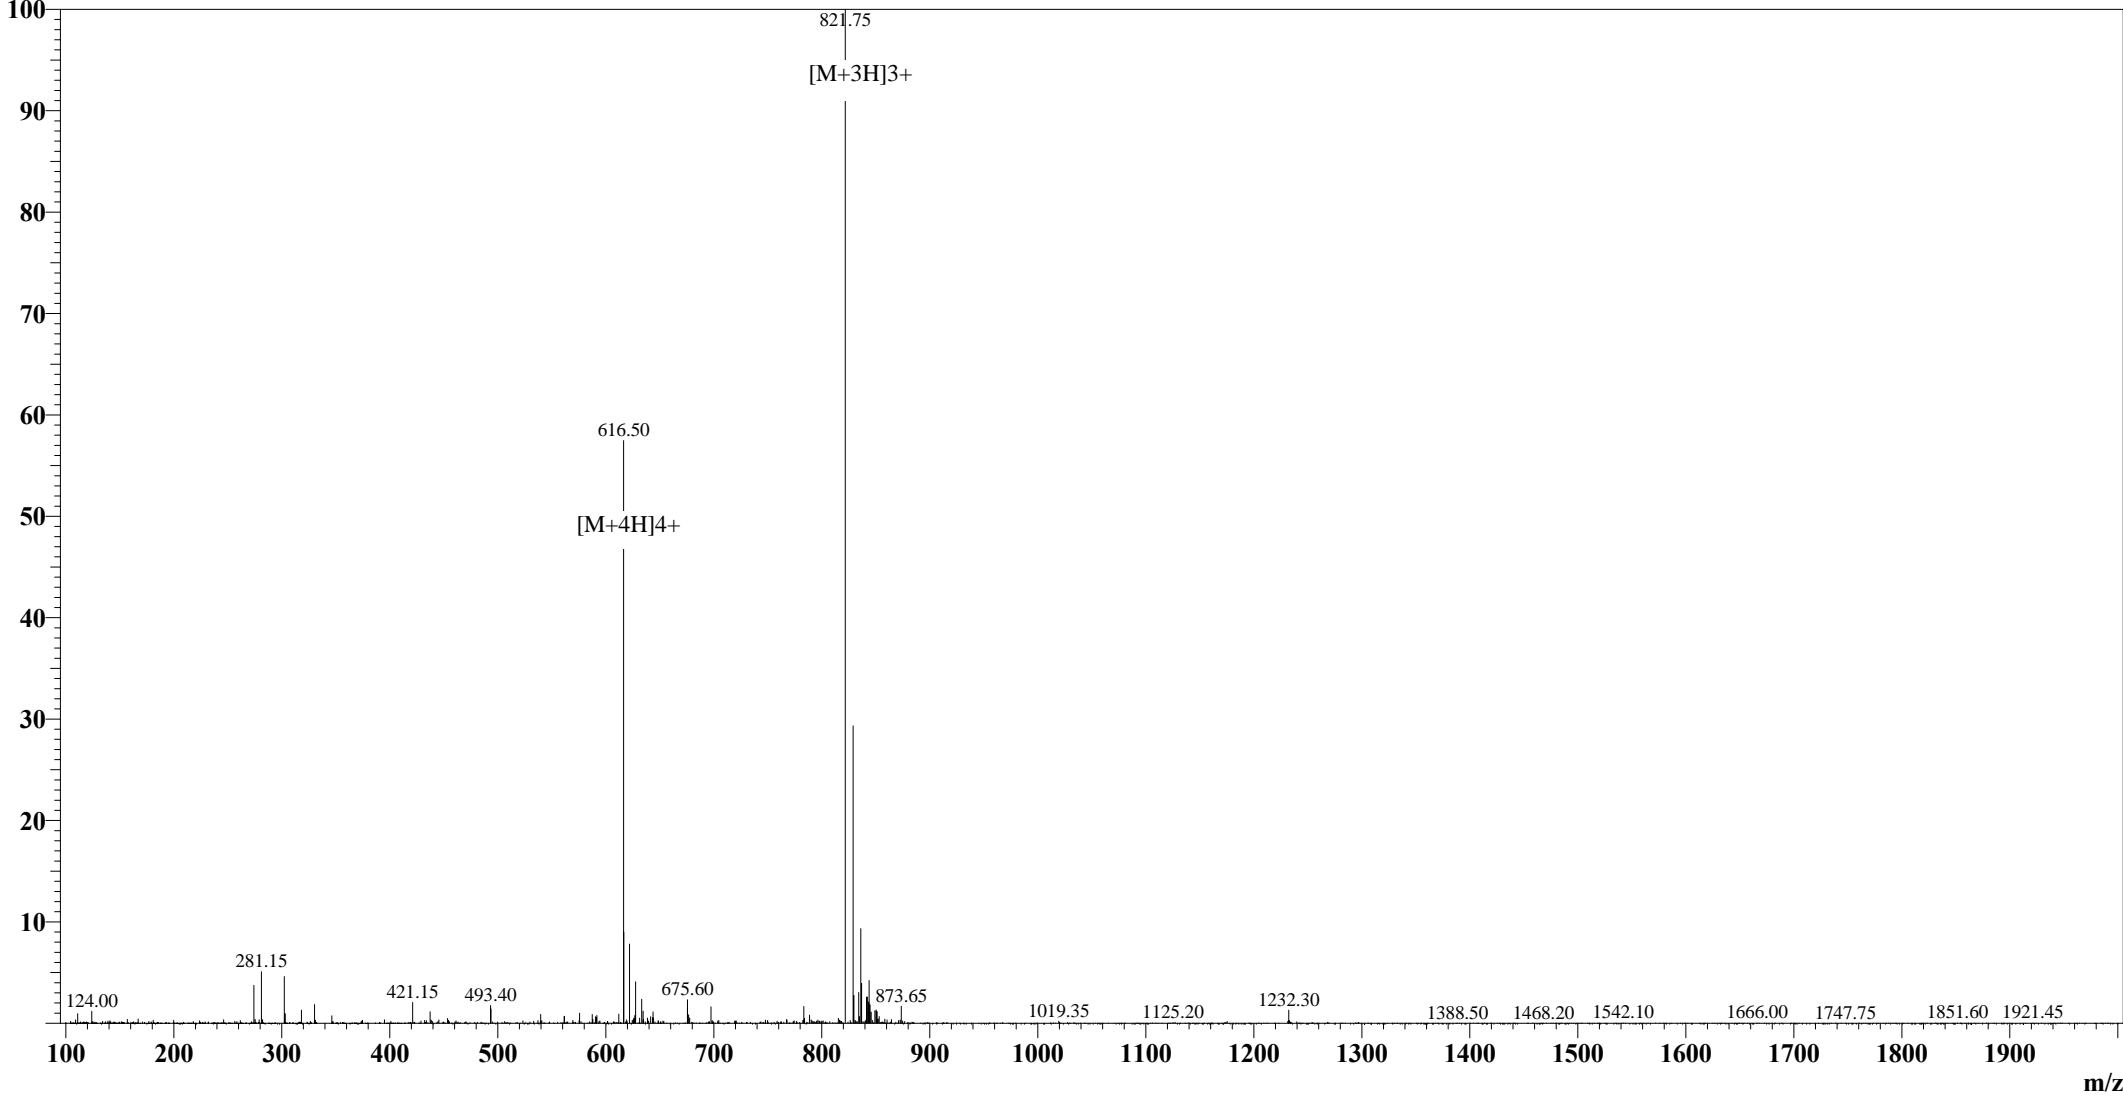

Sample Information

User : Grace
Date Acquired : 12/23/2009 15:03:06
Sample Name : β -Amyloid (1-20)
Cat No. : RP20162S
Lot No. : 86337002122209WJ
Injection Volum : 1.000 μ L
Theoretical MW : 2461.66
Observed MW : 2462.25

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250 $^{\circ}$ C
CDL Volt : -25.0V
Block Temp : 200 $^{\circ}$ C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH