

Sample Name : Biotin-TAT (47-57)
Cat. No. : RP20408
Lot. No. : 86410005122309WJ

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow : 1 ml / min


Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

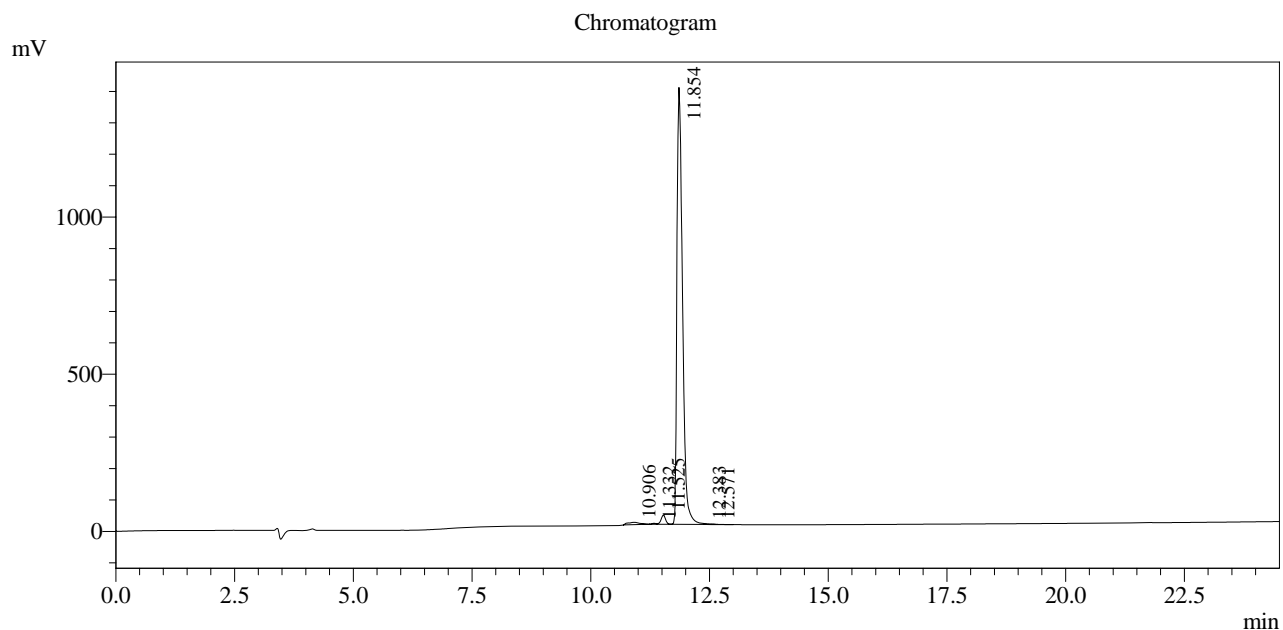

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.906	133908	7427	1.145
2	11.332	19020	3047	0.163
3	11.525	192104	29270	1.643
4	11.854	11306580	1390268	96.712
5	12.383	22701	3127	0.194
6	12.571	16704	1879	0.143
Total		11691016	1435018	100.000