

Sample Name : MAGE-A3 (195-203)
 Cat. No. : RP20413
 Lot. No. : 86410008122309LQ

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow : 1 ml / min

Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

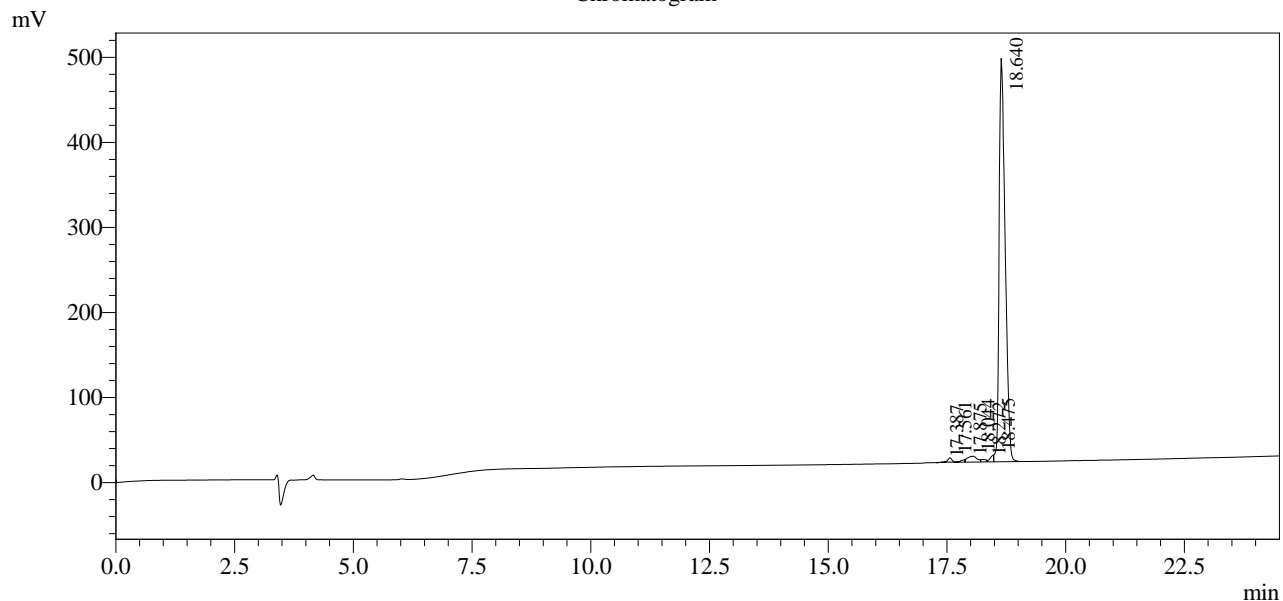

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.387	2067	440	0.047
2	17.561	29051	5112	0.661
3	17.875	16457	2802	0.374
4	18.044	94844	6767	2.158
5	18.272	21433	2859	0.488
6	18.475	39464	7905	0.898
7	18.640	4192369	474274	95.375
Total		4395685	500160	100.000