

Sample Name : Urotensin II, human  
Cat. No. : RP10096  
Lot. No. : 83939001112309WJ

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow : 1 ml / min

Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

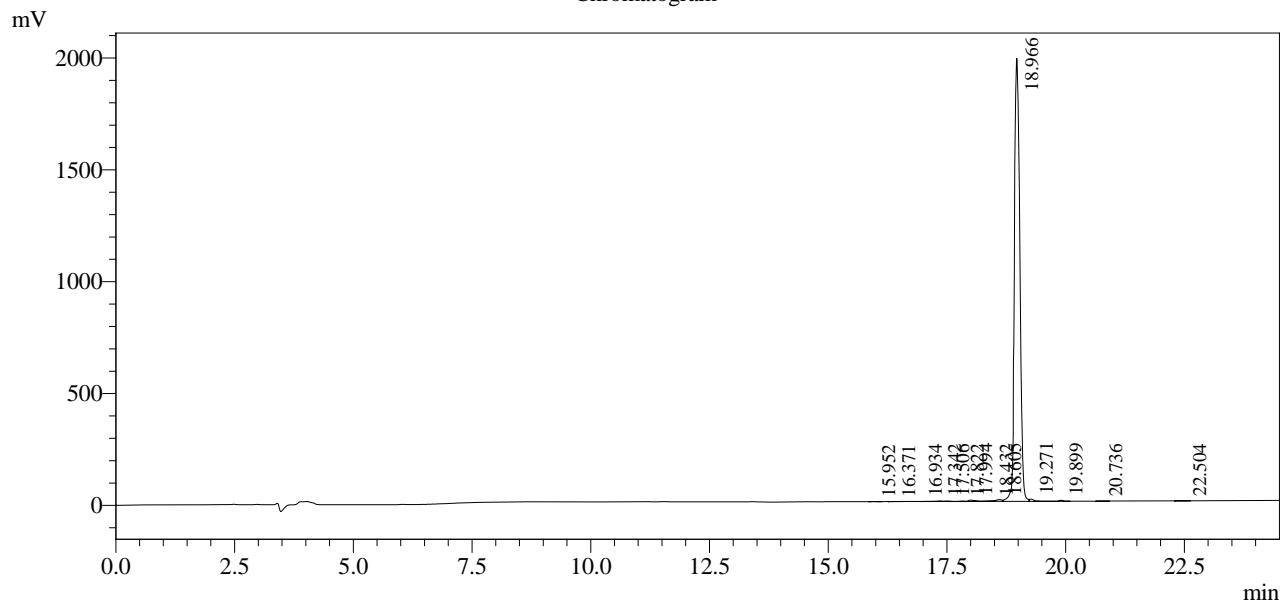

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.952	5157	676	0.032
2	16.371	8493	668	0.052
3	16.934	15607	1946	0.096
4	17.342	25330	2662	0.156
5	17.506	21831	2302	0.135
6	17.822	19244	2226	0.119
7	17.994	70884	6045	0.437
8	18.432	24866	3150	0.153
9	18.605	69277	8171	0.427
10	18.966	15844791	1980068	97.691
11	19.271	70497	9954	0.435
12	19.899	25700	4300	0.158
13	20.736	6459	957	0.040
14	22.504	11085	1514	0.068
Total		16219220	2024638	100.000