

Sample Name : OVA G4 peptide
Cat. No. :RP20398
Lot. No. :84280008112509ZW

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

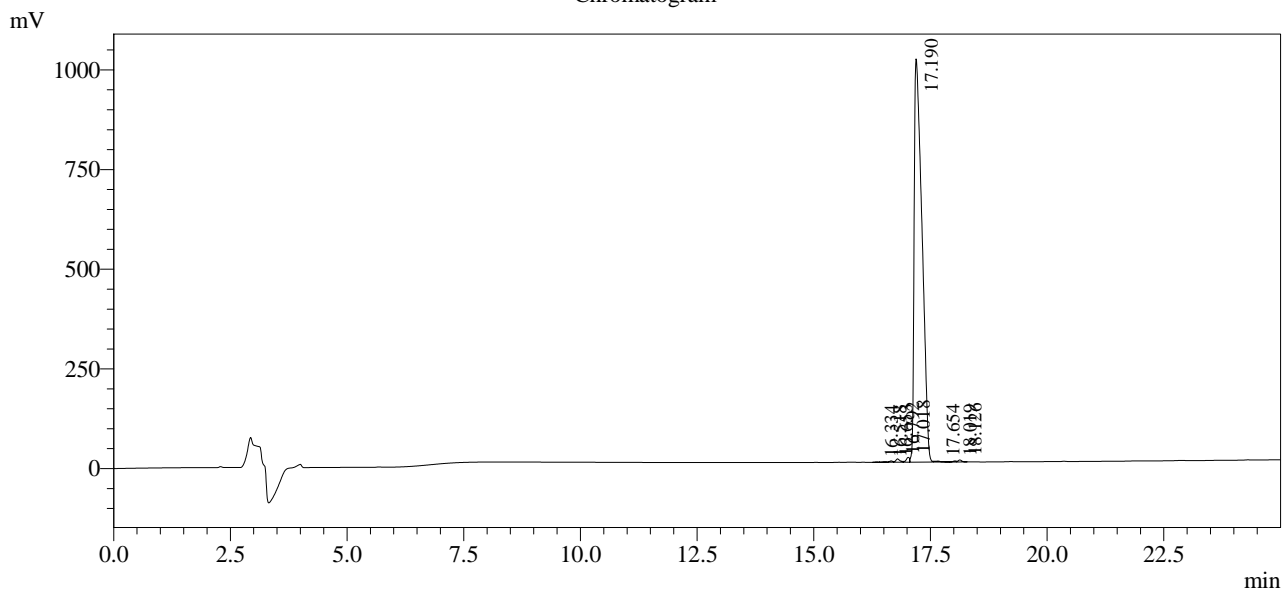

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.334	2891	599	0.024
2	16.518	6505	983	0.054
3	16.653	17807	3295	0.148
4	16.792	51542	8328	0.429
5	17.018	60489	11932	0.504
6	17.190	11802855	1011558	98.312
7	17.654	23754	2446	0.198
8	18.019	13720	2685	0.114
9	18.126	25893	5050	0.216
Total		12005456	1046876	100.000