

Sample Name : Transdermal Peptide
 Cat. No. :RP20404
 Lot. No. :88893002012910ZW


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

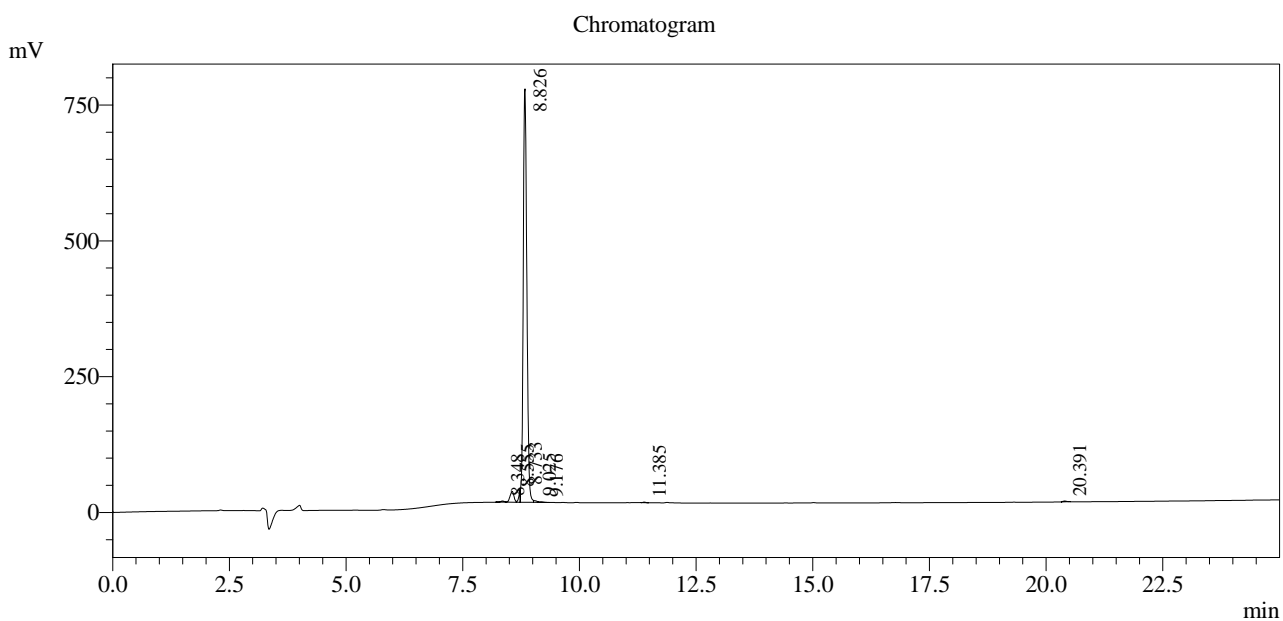

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.348	12692	2132	0.294
2	8.555	115948	20061	2.688
3	8.733	51525	23786	1.195
4	8.826	4098022	761091	95.013
5	9.025	14908	3319	0.346
6	9.176	7523	1138	0.174
7	11.385	4506	1086	0.104
8	20.391	7989	1479	0.185
Total		4313113	814092	100.000