


Positive

MS Spectrum

Intensity

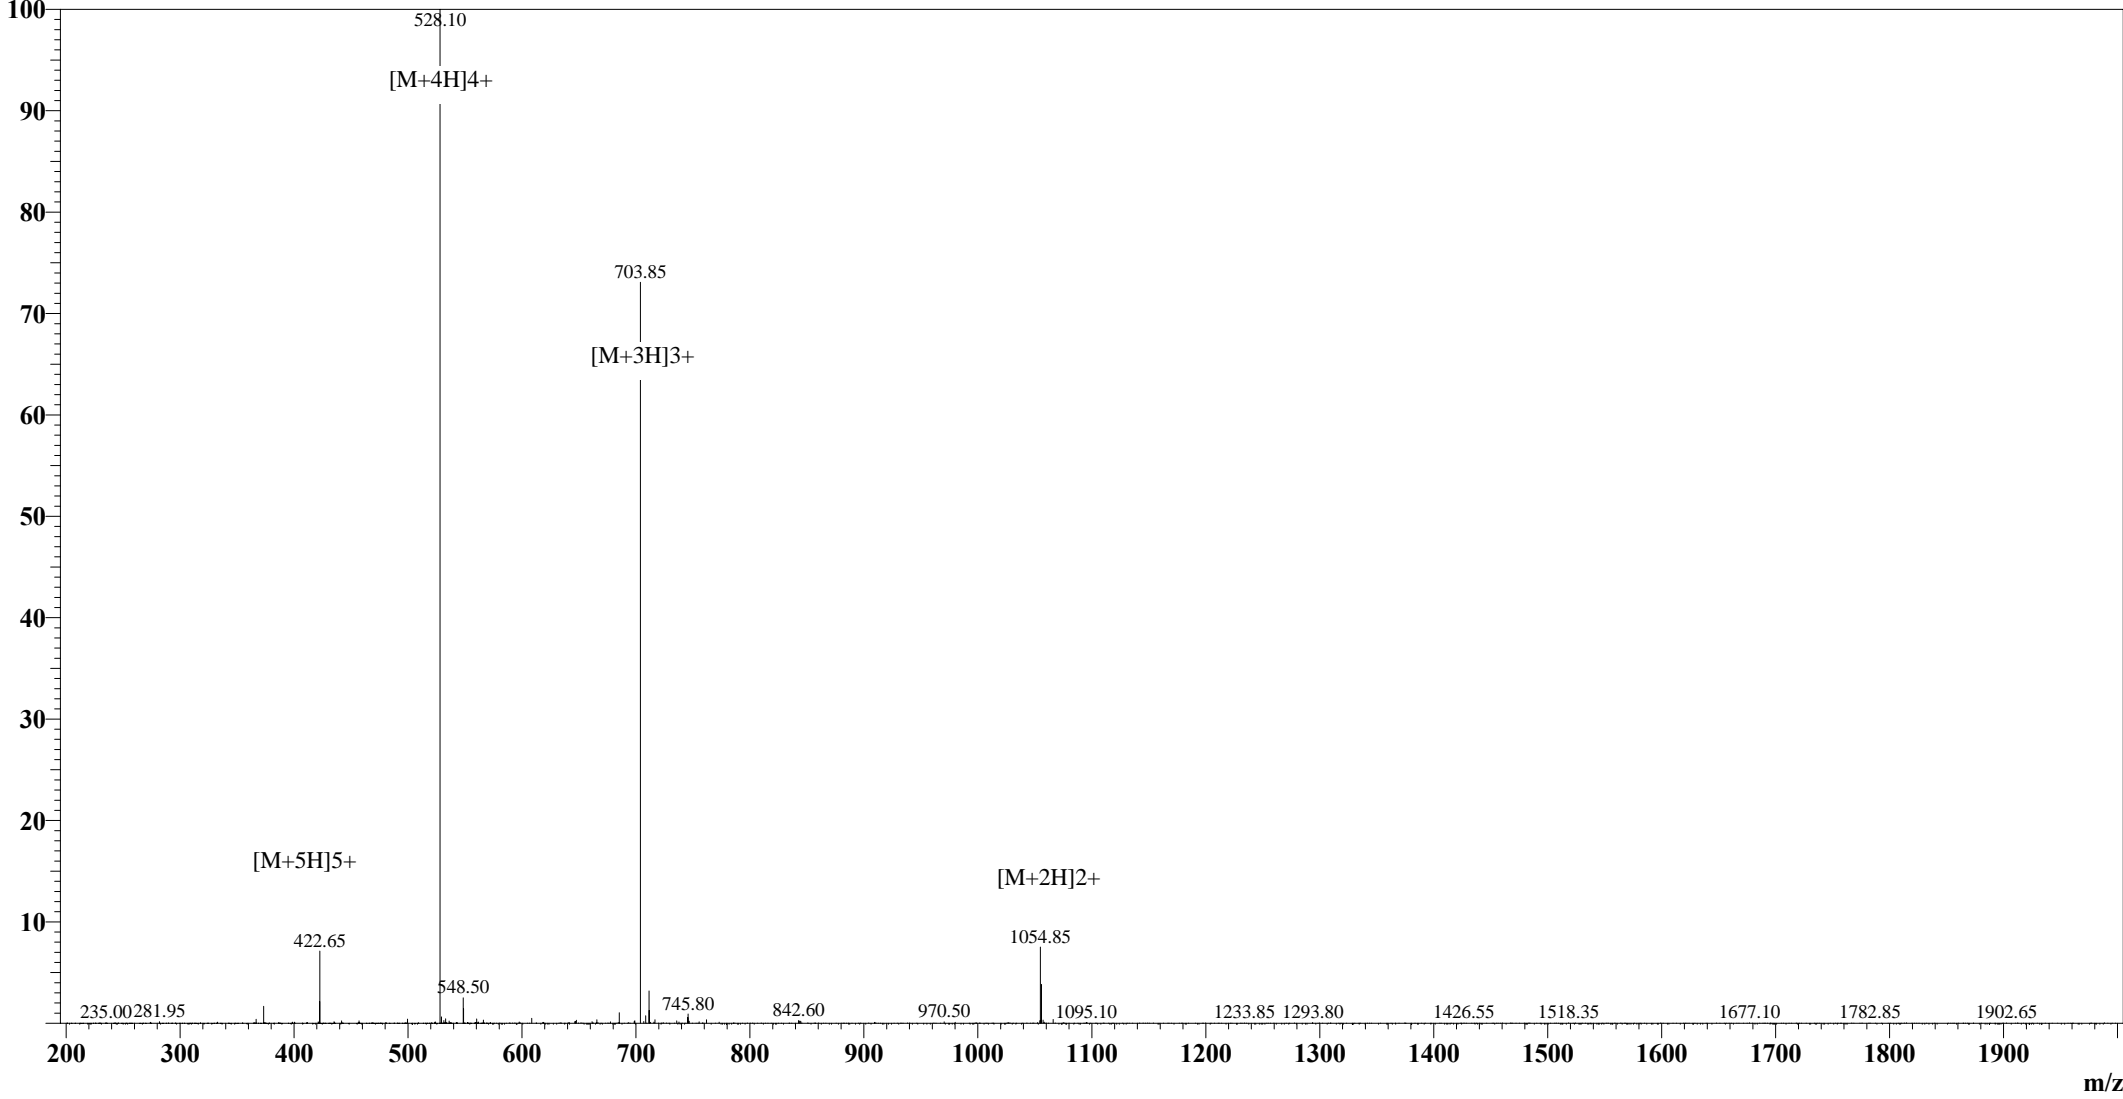

Sample Information

User : Grace
Date Acquired : 01/22/2010 15:31:35
Sample Name : Apidaecin IB
Cat No. : RP20409
Lot No. : 88893004012910ZW
Injection Volum : 1.000µL
Theoretical MW : 2108.40
Observed MW : 2108.55

Interface : ESI
Nebulizing Gas Flow : 4.21 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH