


Positive

MS Spectrum

Intensity

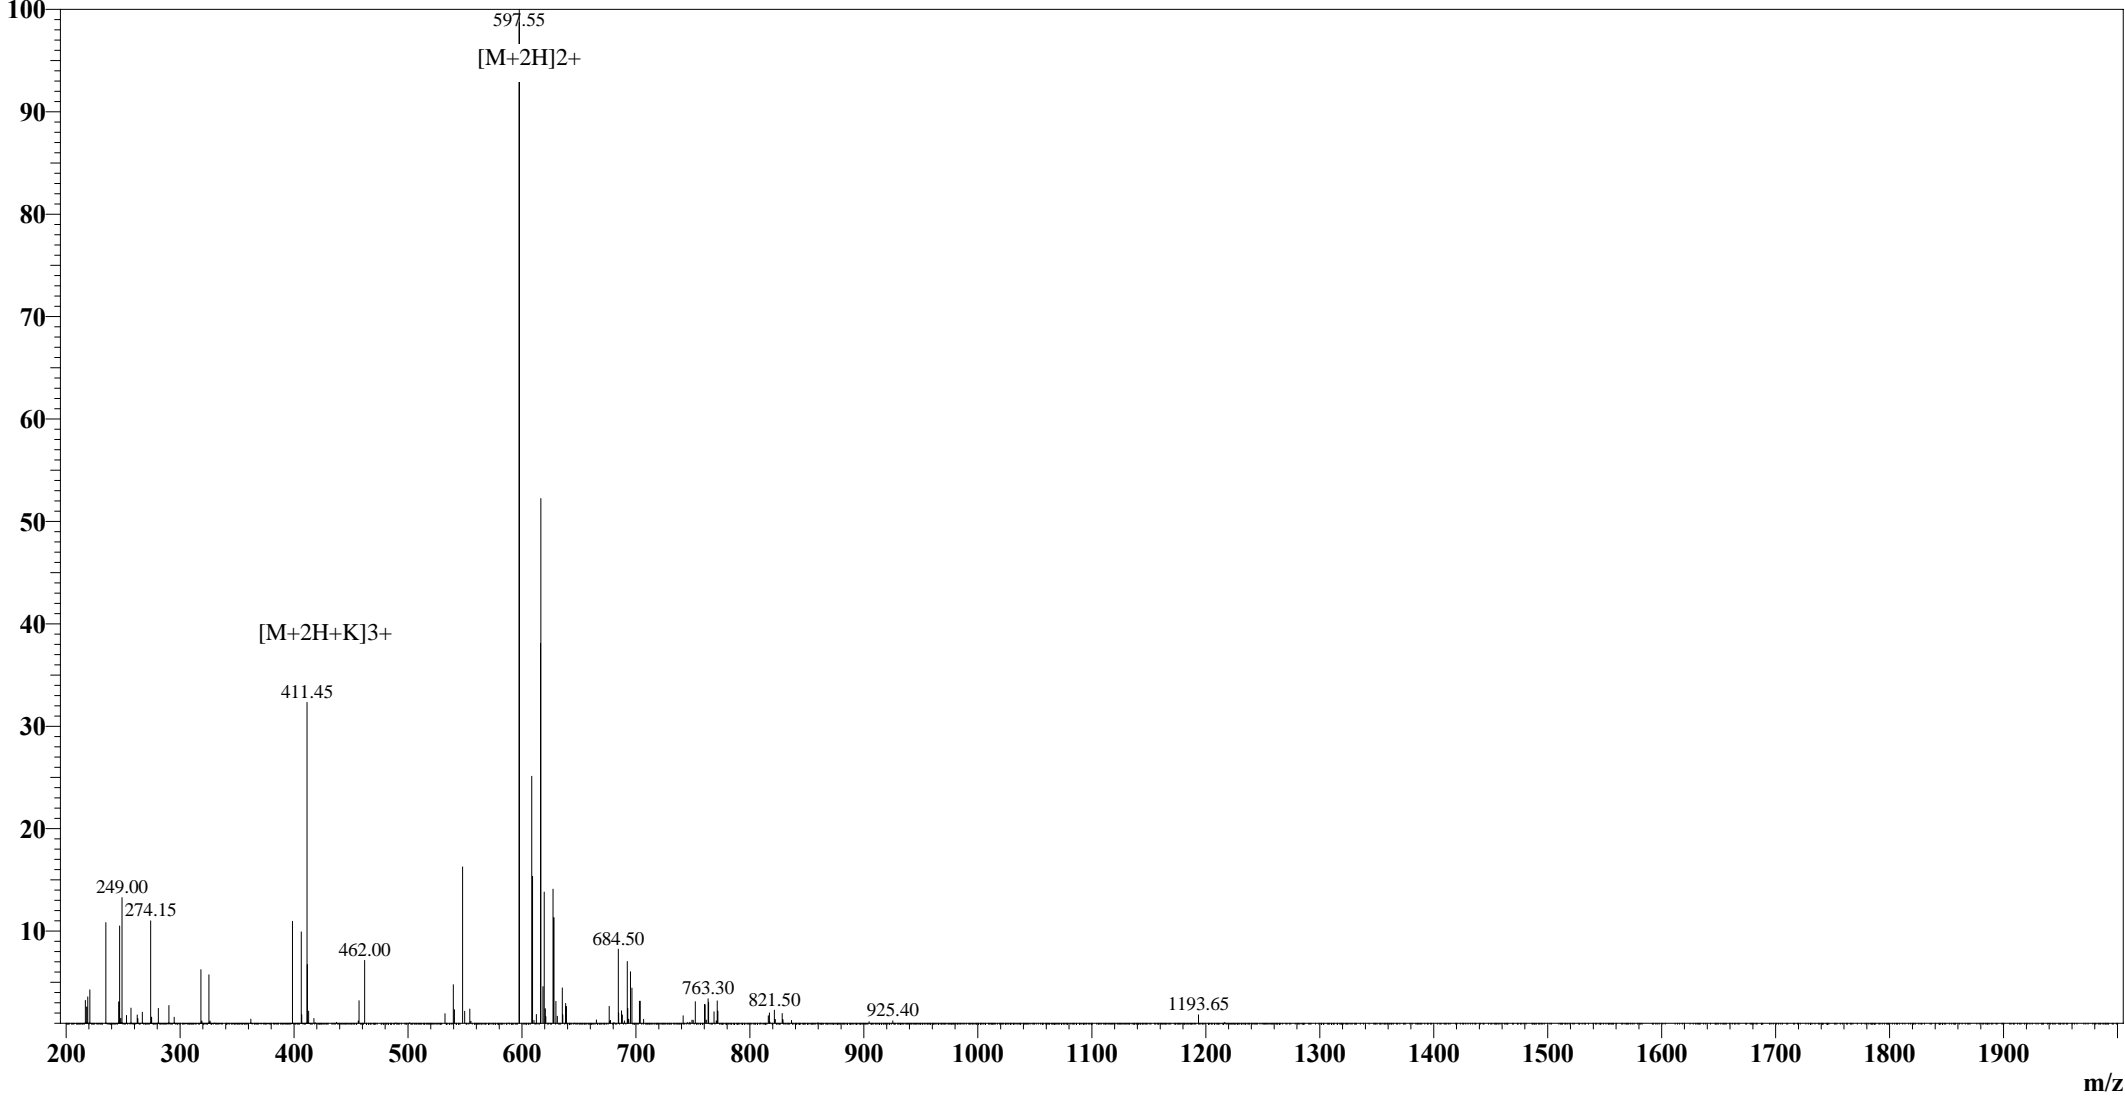

Sample Information

User : Grace  
Date Acquired : 01/04/2010 13:23:27  
Sample Name : CEF7, Influenza Virus NP (380-388)  
Cat No. : RP20419  
Lot No. : 88893007012910ZW  
Injection Volum : 1.000µL  
Theoretical MW : 1193.40  
Observed MW : 1193.10

Interface : ESI  
Nebulizing Gas Flow : 4.21 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias : +4.5kv  
Detector : 1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH