

Sample Name :Competence-Stimulating Peptide-12261
Cat. No. :RP20427
Lot. No. :88894002012910BF

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

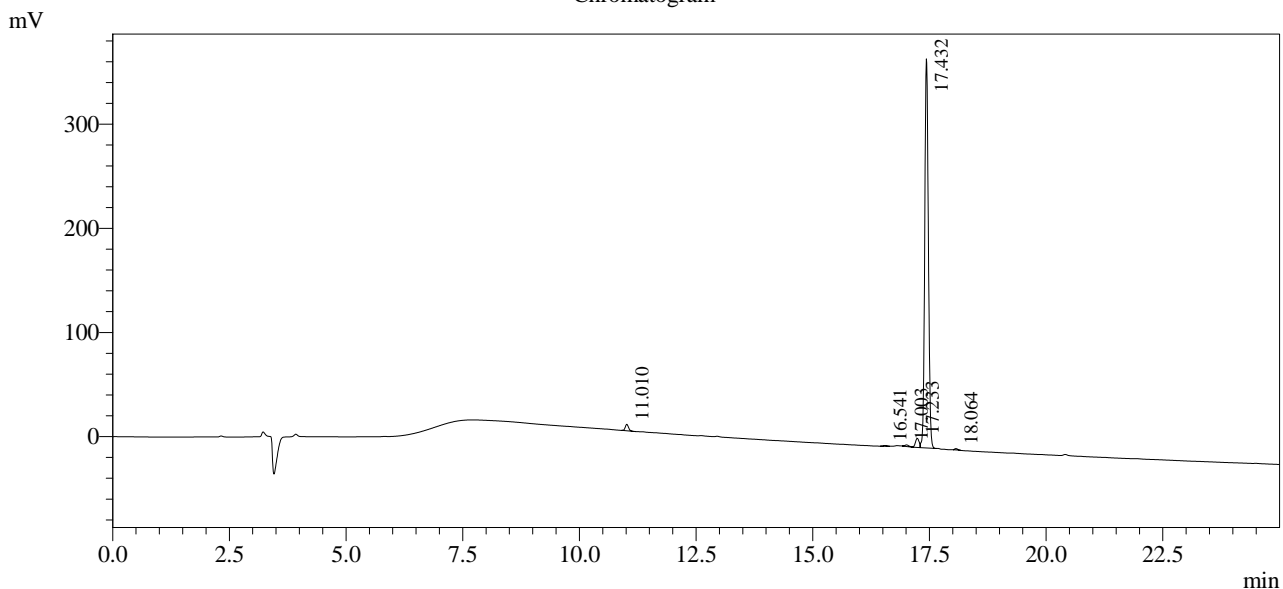

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.010	30488	6251	1.432
2	16.541	2669	562	0.125
3	17.003	8593	1478	0.404
4	17.233	47486	8733	2.231
5	17.432	2034135	373630	95.549
6	18.064	5521	1273	0.259
Total		2128891	391927	100.000