


Positive

M/S Spectrum

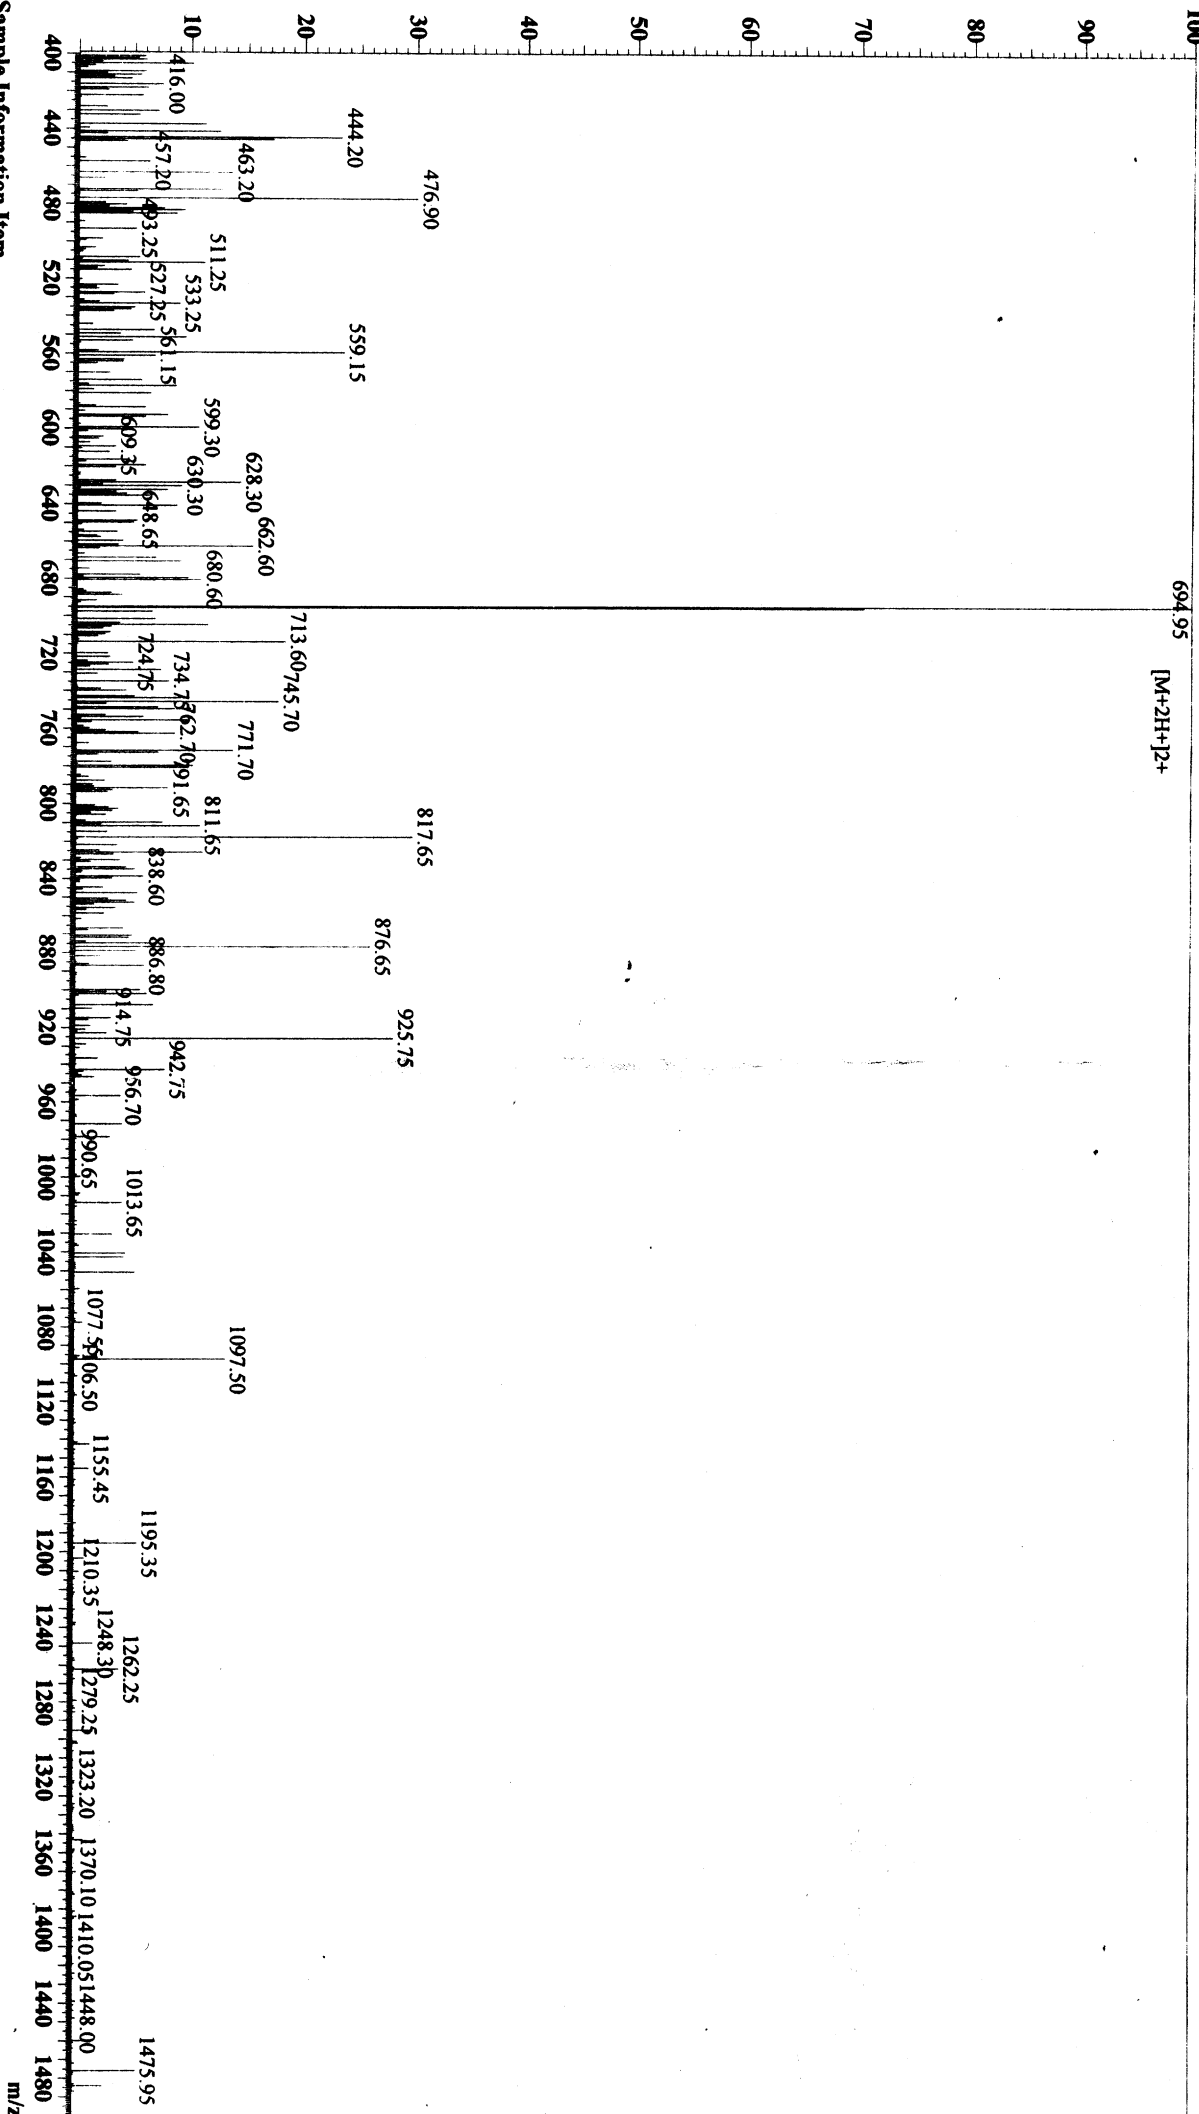

Sample Information Item

Date and Time : 2005-5-21 15:38:10

User : FJS

Sample : EV-11(O)

Ini. Volume : 1.000

MTW : 1388.60

Cat. No.: RP10096

Lot No.: PX00109510

Probe:

Nebulizer Gas Flow:

CDL:

Block Temp:

ESI

1.5L/min

-20.0V

250°C

Probe bias:

Detector:

T. Flow:

B. conc:

+4.5kV

1.5kV

0.2ml/min

50% H_2O /50%ACN