


MS Spectrum

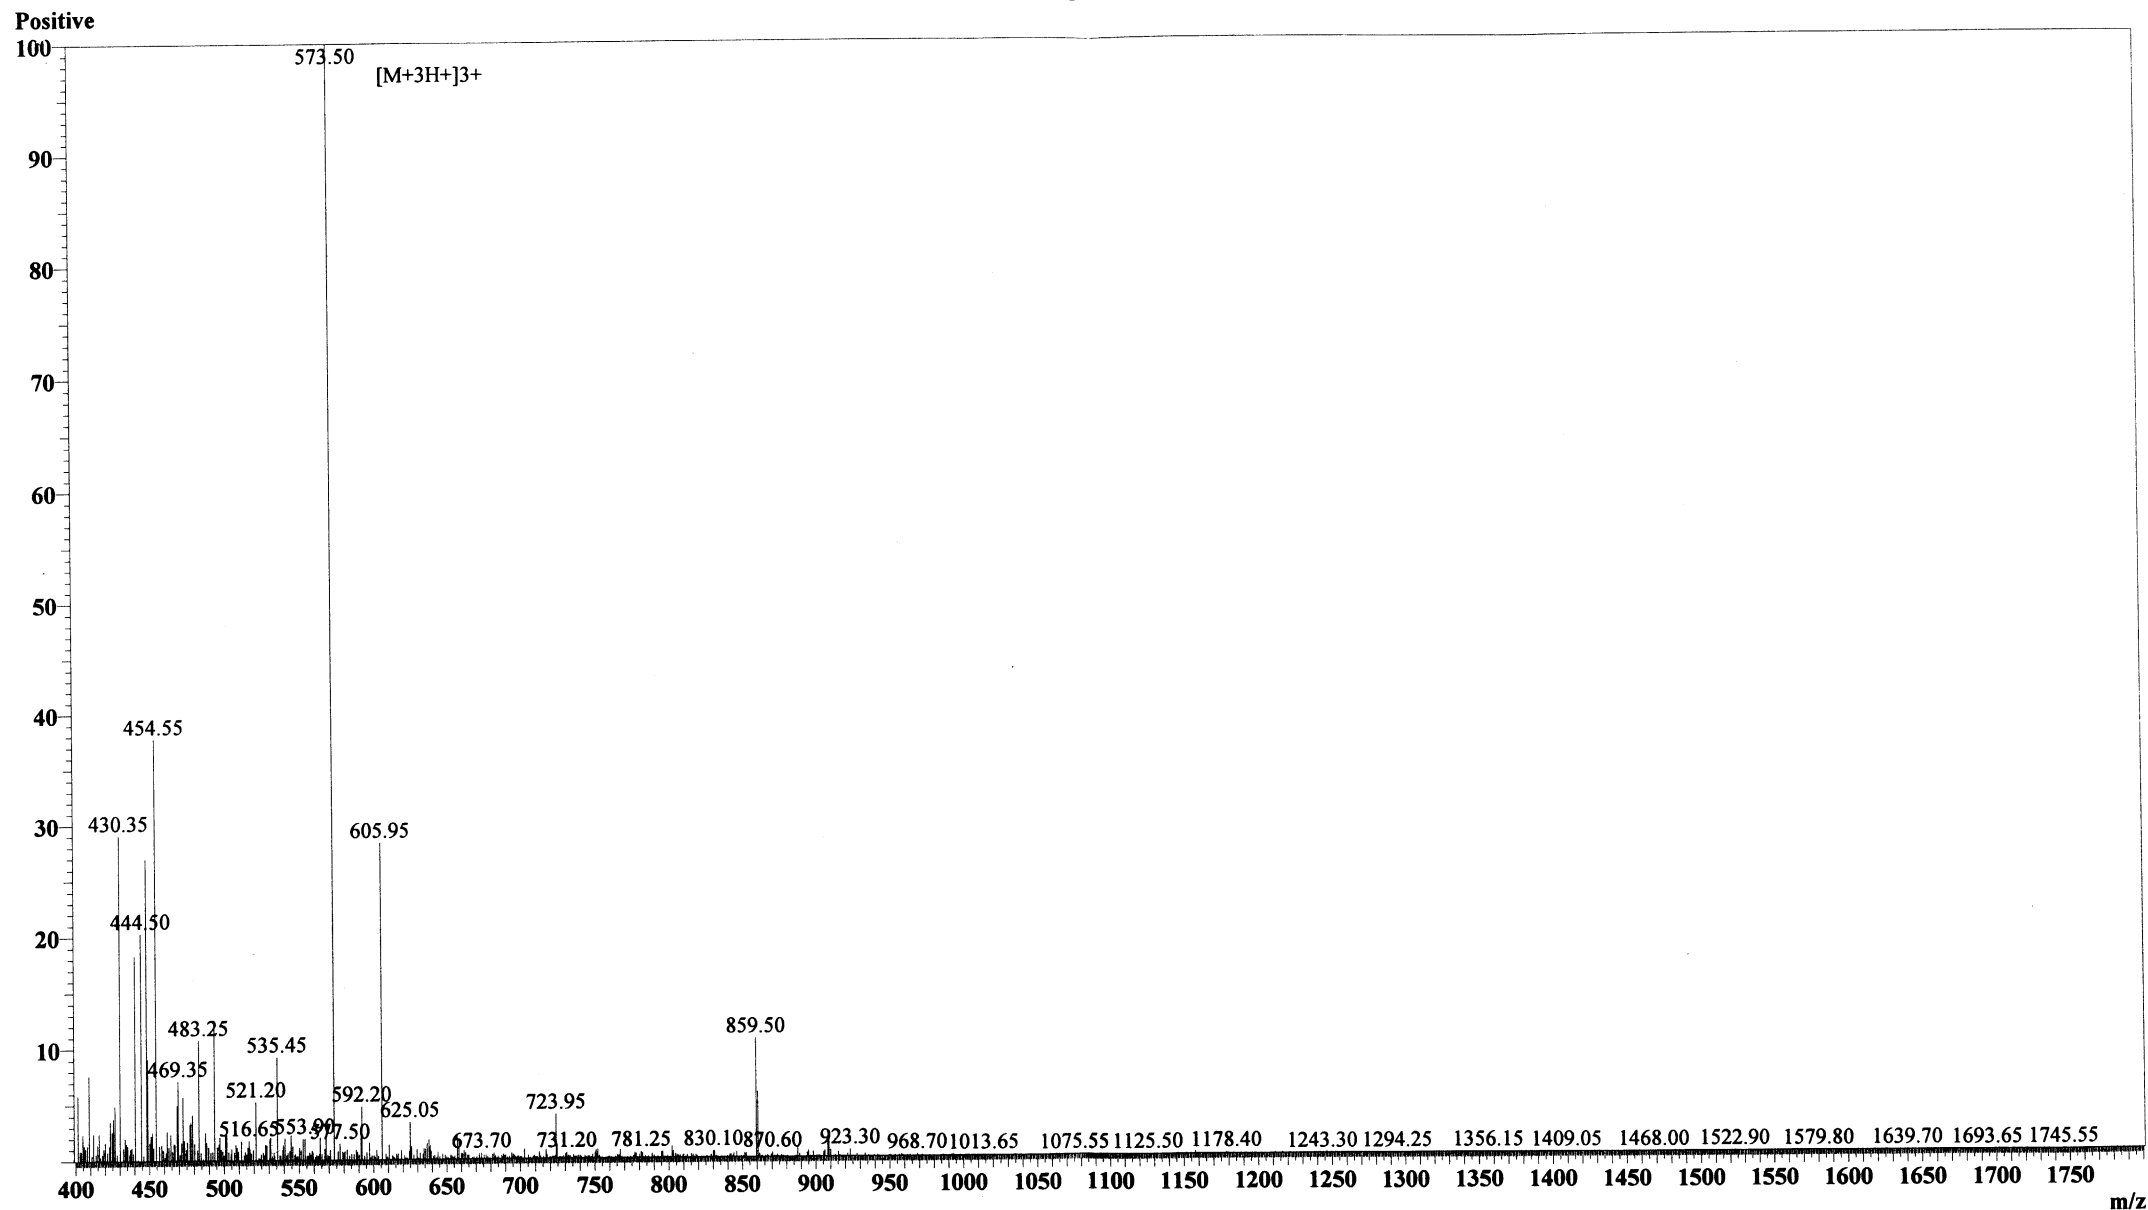

Sample Information Item

Date and Time : 2005-4-1 15:53:52
 User : xie
 Sample : RP10142(KR-13)
 Inj. Volume : 1.000
 MW : 1717.03

Cat No.: RP10142
 Lot No.: PJ00508506

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp: 250°C
 Block Temp: 200°C

Probe bias: +4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. conc: 50%H2O/50%ACN