


MS Spectrum

Positive

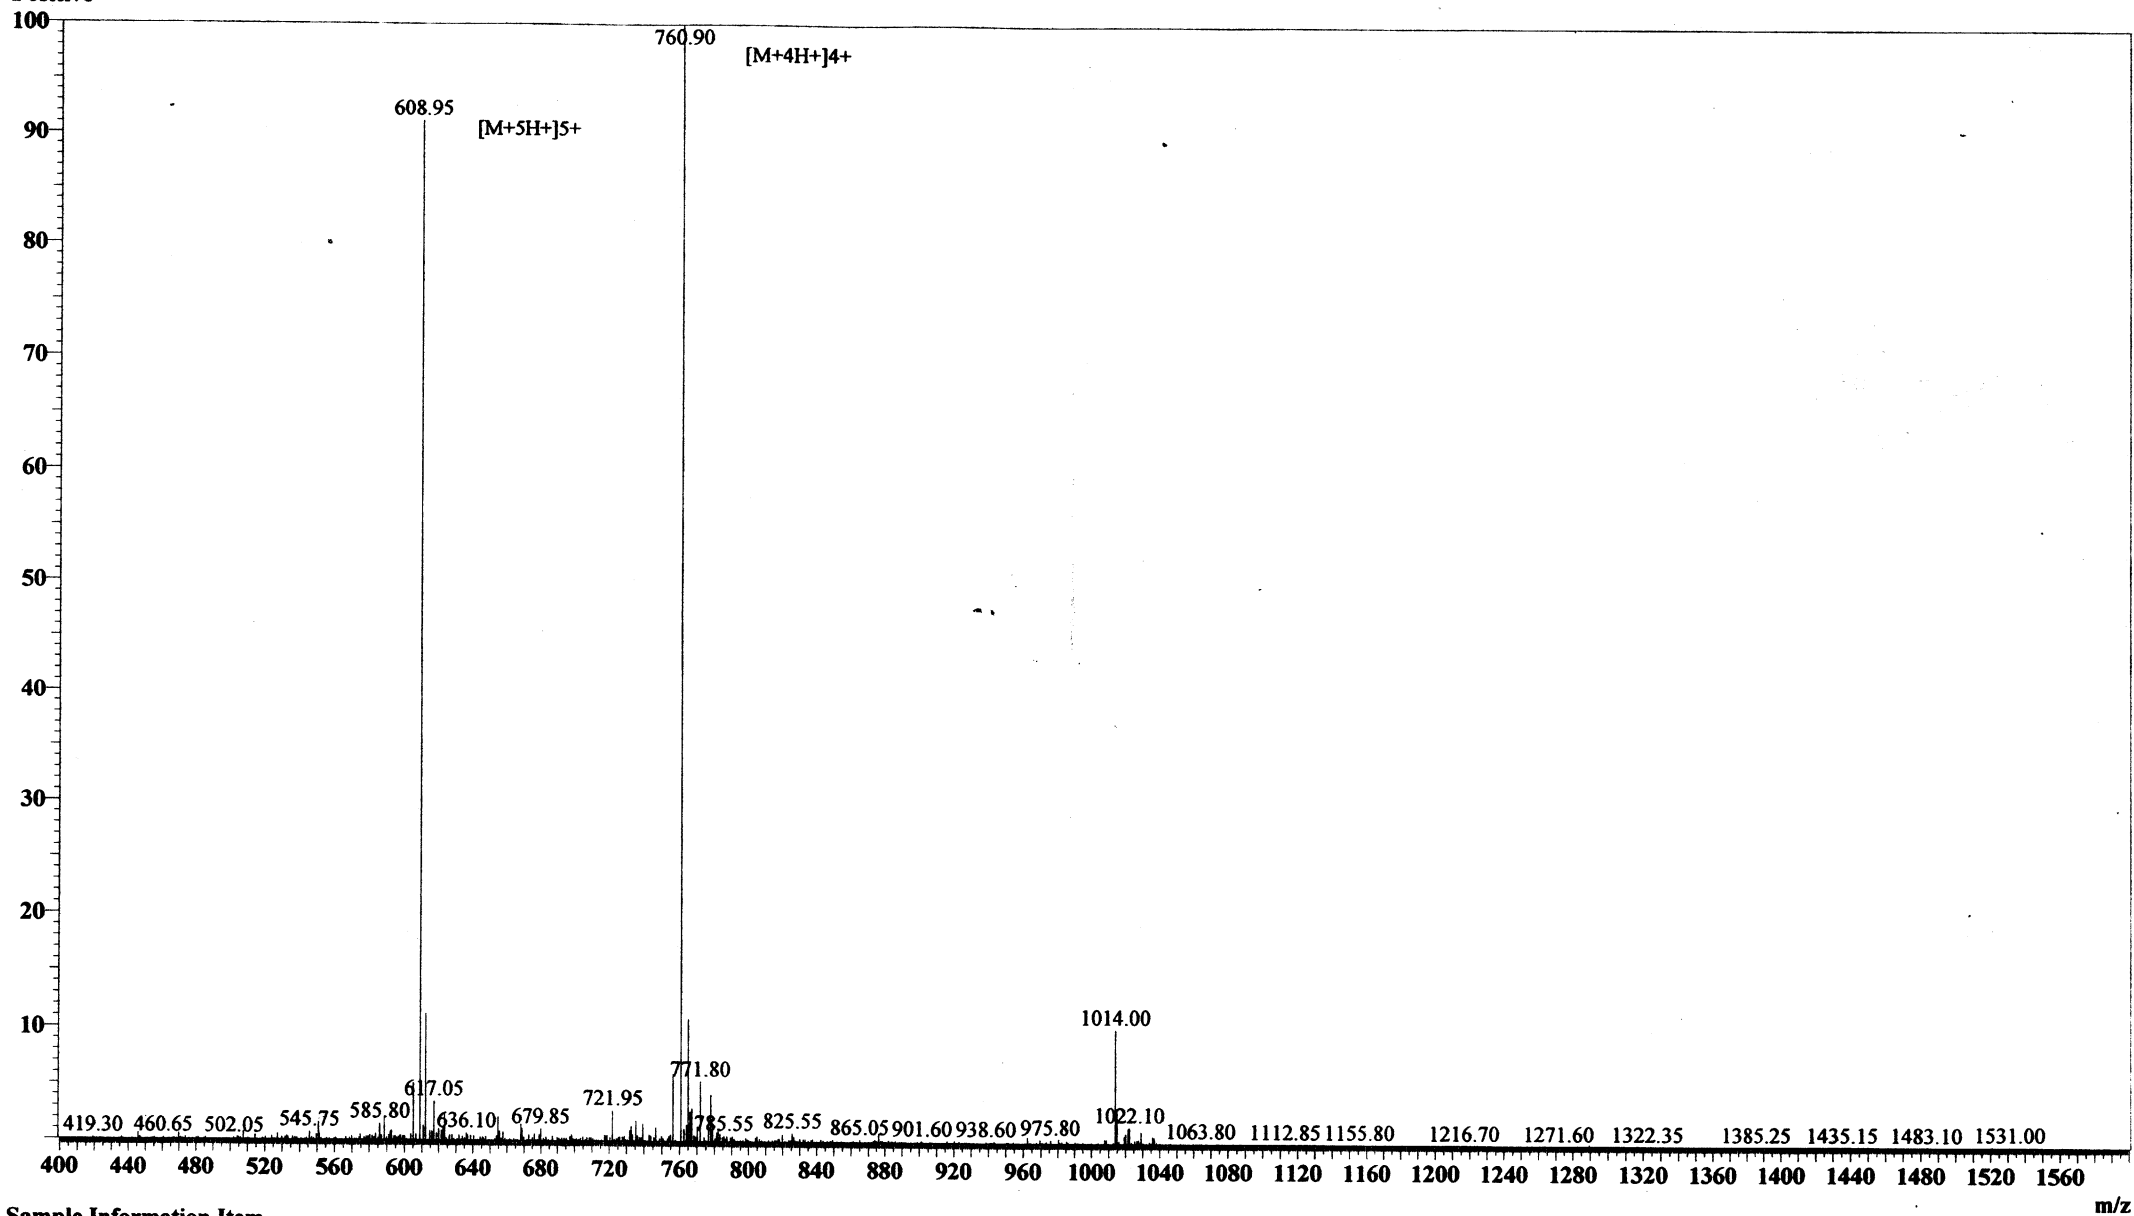

m/z

Sample Information Item

Date and Time : 2005-5-10 18:12:00
User : FJS
Sample : HV-27-NH2-1
Inj. Volume : 1.000
MW : 3039.47

Cat. No.: RP10249

Lot No.: PX00209510

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN