


Positive

MS Spectrum

Intensity

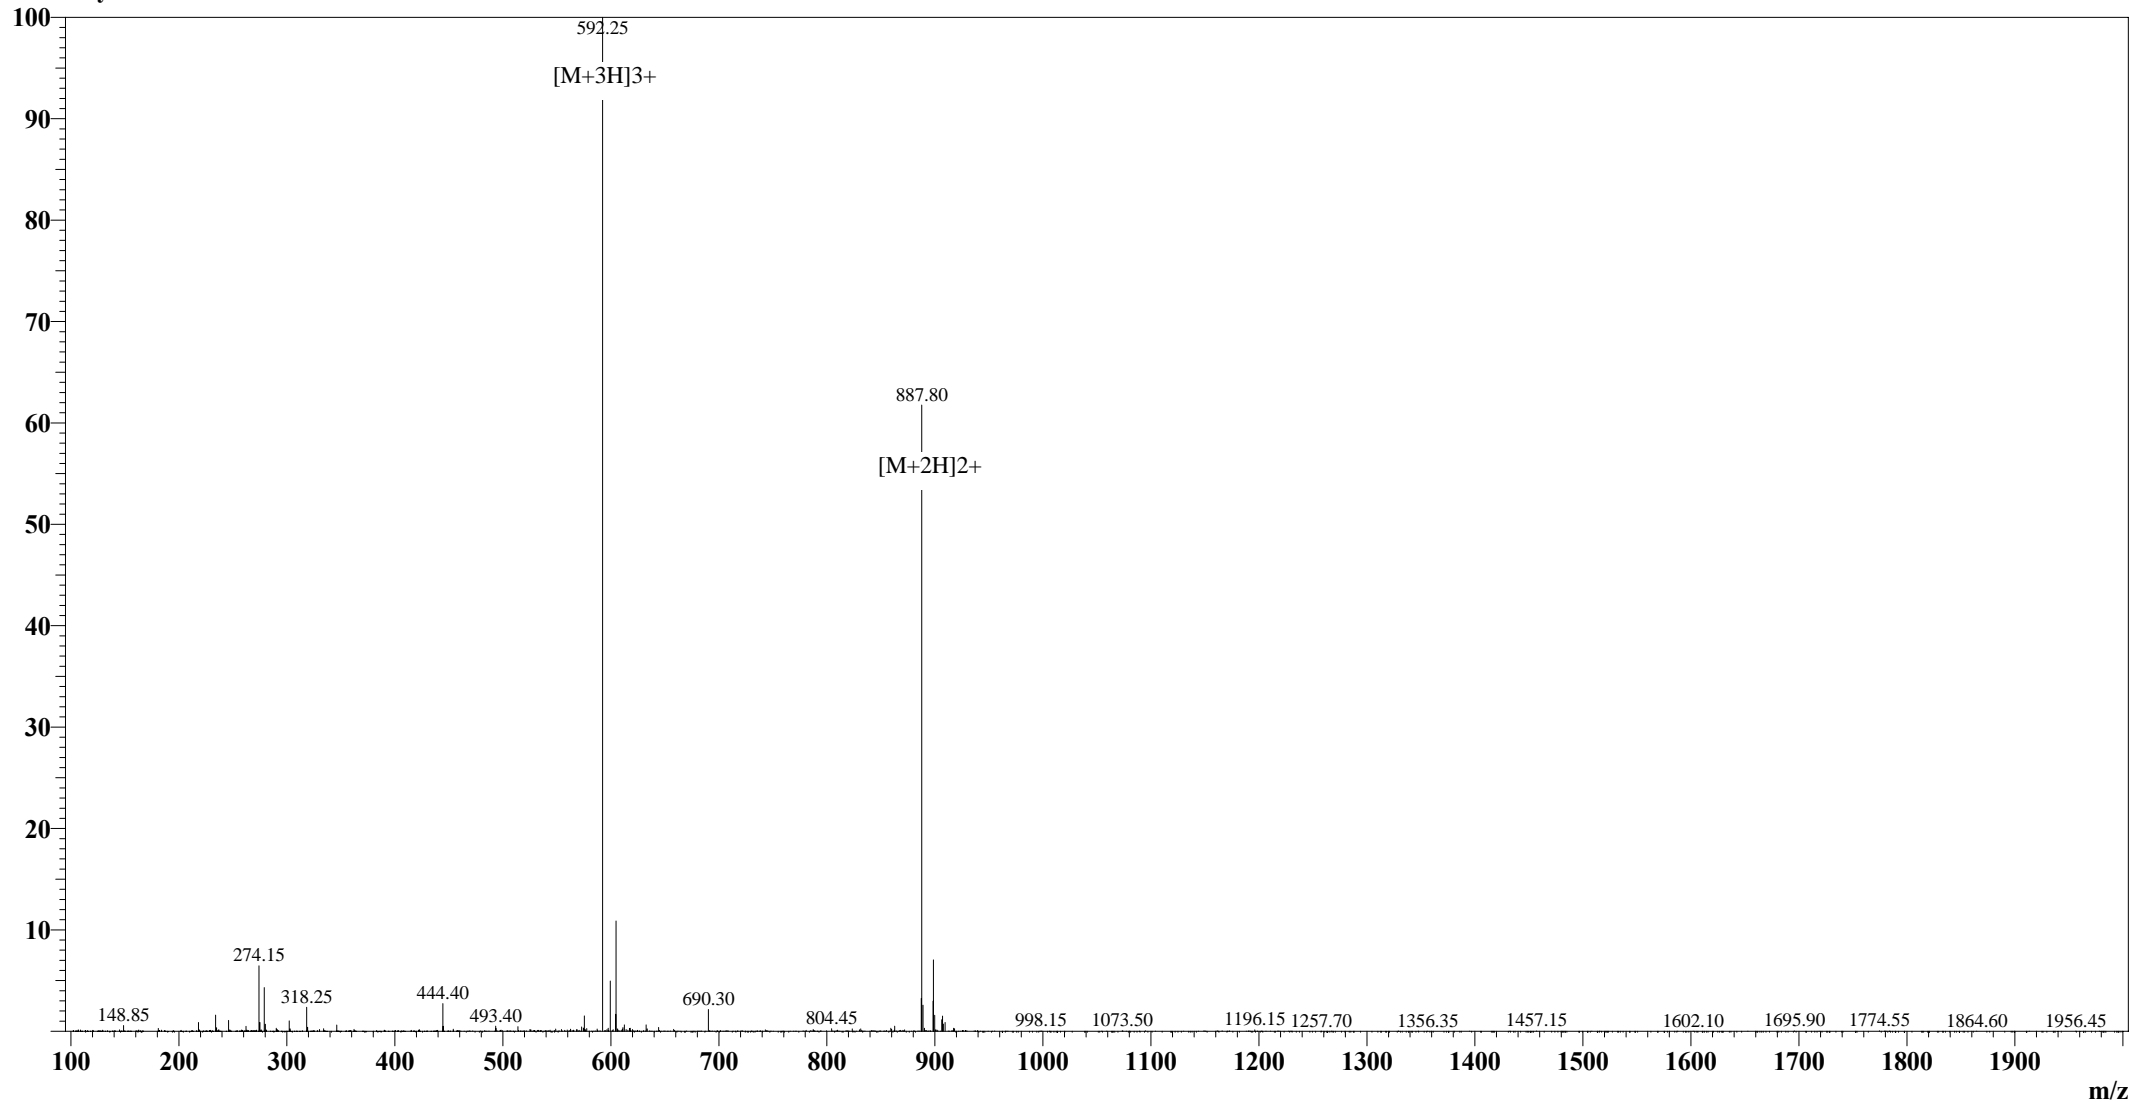

Sample Information

User : Grace
Date Acquired : 06/21/2009 21:37:42
Sample Name : OVA Peptide (323-339)
Cat No. : RP10610
Lot No. : CC10906
Injection Volum : 1.000µL
Theoretical MW : 1772.94
Observed MW : 1773.60

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH