


MS Spectrum

Positive

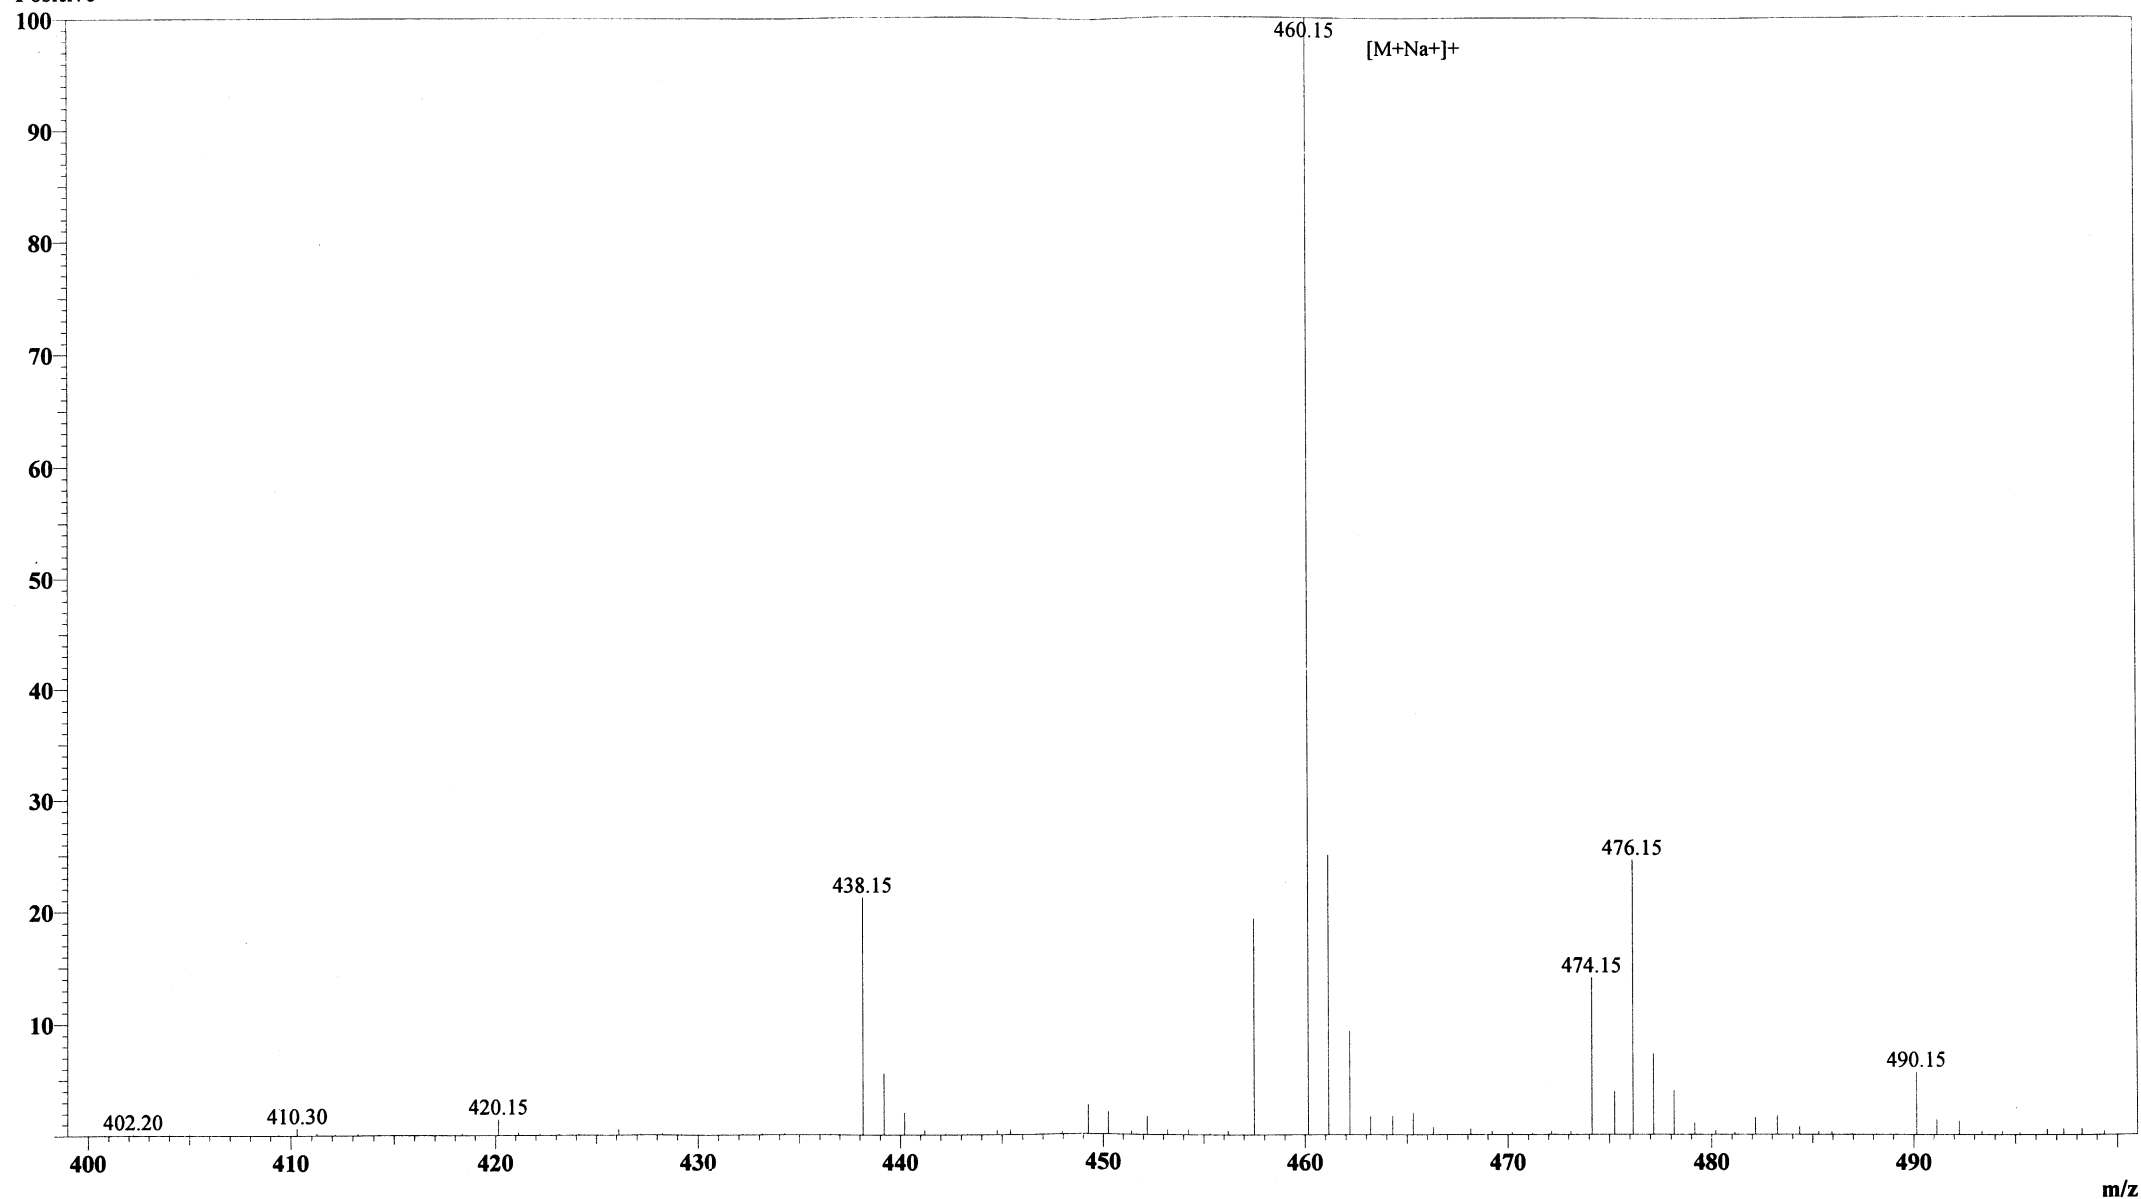

Sample Information Item

Date and Time : 2005-5-25 19:03:04
 User : FJS
 Sample : For-MF-3
 Inj. Volume : 1.000
 MW : 437.56

Cat. No.: RP12956

Lot No.: PJ01106506

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp: 250°C
 Block Temp: 200°C

Probe bias: +4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. conc: 50%H2O/50%ACN