


MS Spectrum

Positive

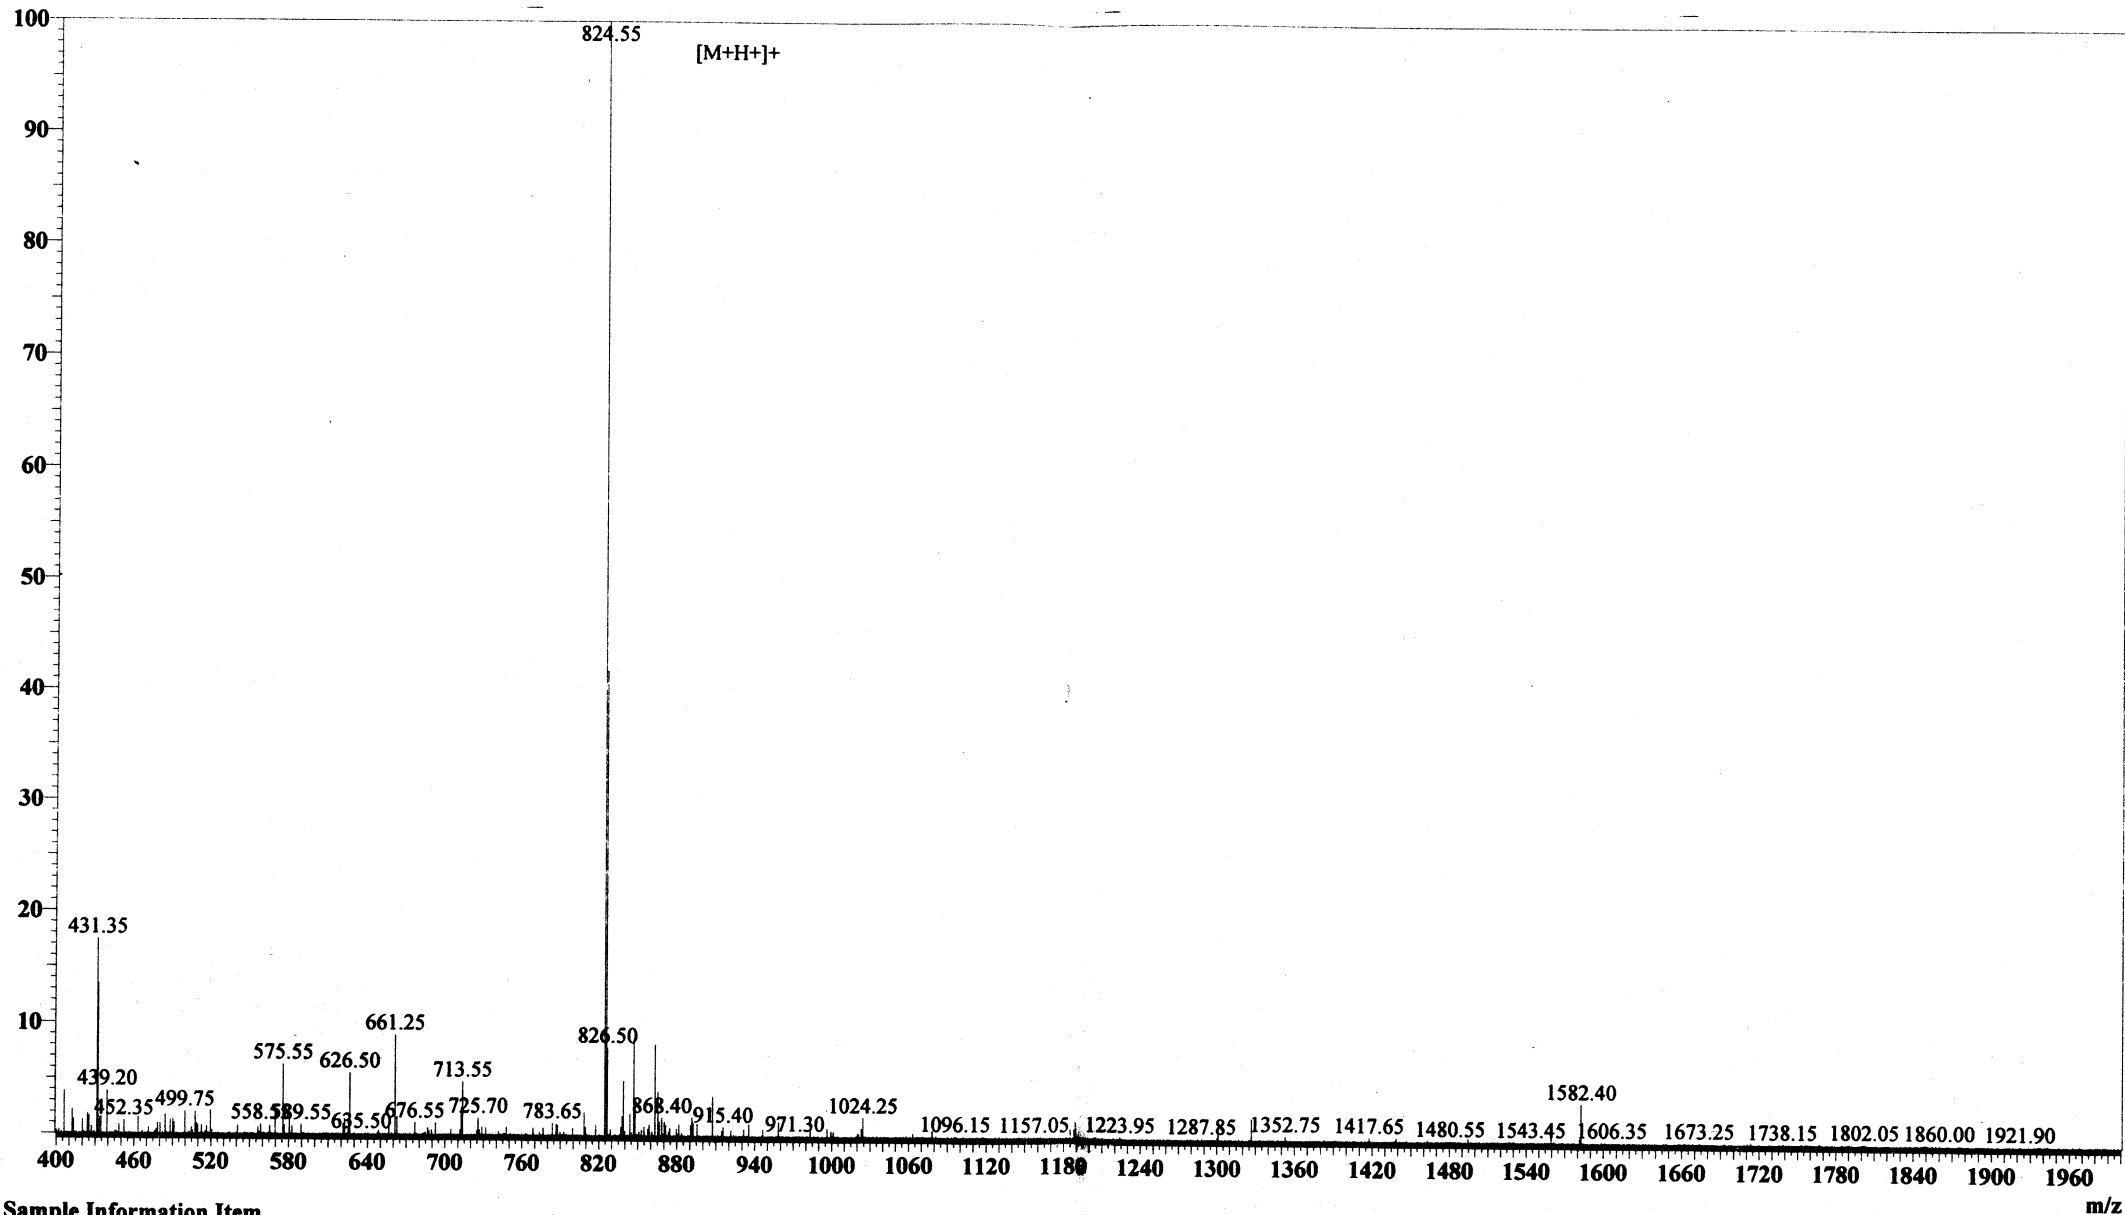

Sample Information Item

Date and Time : 2005-6-9 21:37:23
 User : FJS
 Sample : RP12959(For-Nle-LK-5)
 Inj. Volume : 1.000
 MW : 824.04

Cat. No.: RP12959

Lot No.: PX00112507

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp: 250°C
 Block Temp: 200°C

Probe bias: +4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. conc: 50%H2O/50%ACN