

Sample Name :  $\beta$ -Amyloid (25-35)  
 Cat. No. : RP10008  
 Lot. No. : CD22907

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow : 1 ml / min  
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

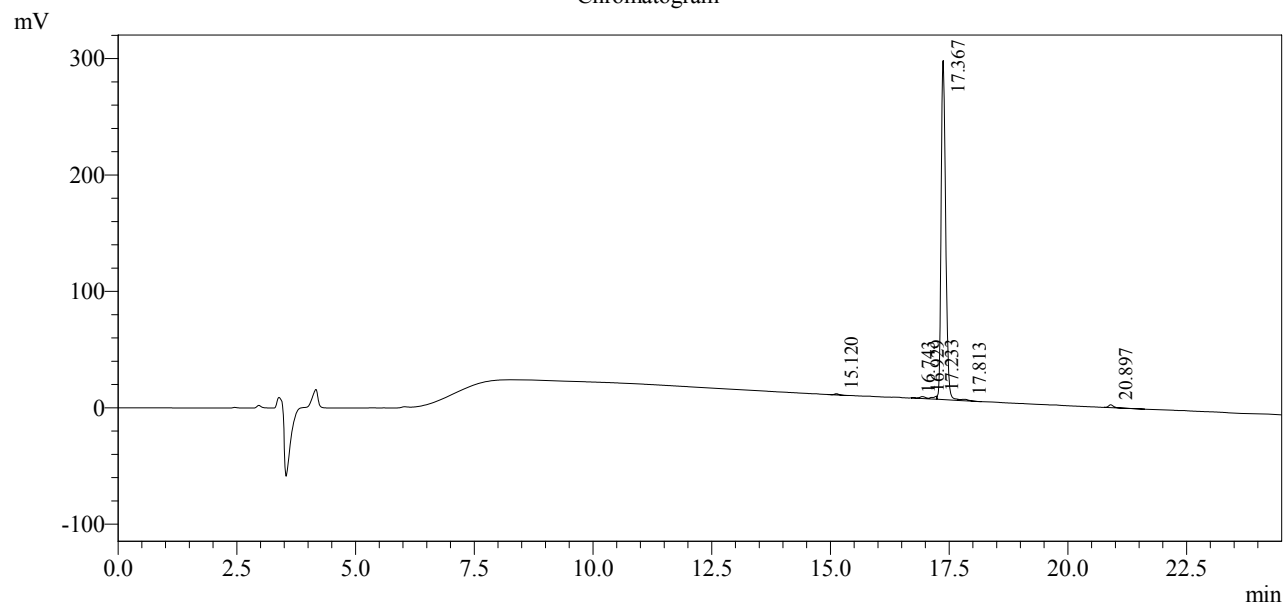

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.120	6125	1023	0.305
2	16.743	1065	238	0.053
3	16.929	12962	1603	0.645
4	17.233	16443	2646	0.818
5	17.367	1938031	291403	96.460
6	17.813	14631	1216	0.728
7	20.897	19890	2490	0.990
Total		2009147	300618	100.000