

Sample Name : MBP
Cat. No. :RP10314
Lot. No. :CC03905


Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:214 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01 | Pumps | Pump A B.Conc | 5 | |
| 25.00 | Pumps | Pump A B.Conc | 65 | |
| 25.10 | Pumps | Pump A B.Conc | 95 | |
| 33.00 | Pumps | Pump A B.Conc | 95 | |
| 33.10 | Pumps | Pump A B.Conc | 5 | |
| 43.00 | Pumps | Pump A B.Conc | 5 | |
| 43.10 | Controller | Stop | | |

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

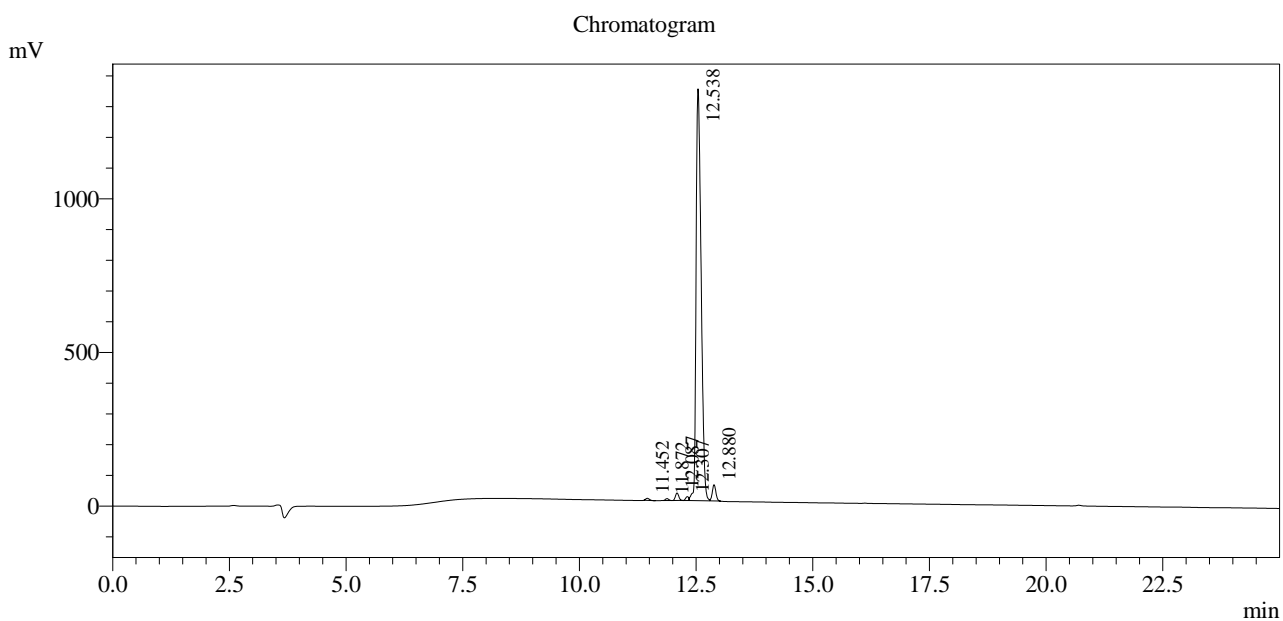

Peak Table

Detector A Ch1 214nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|----------|---------|---------|
| 1 | 11.452 | 36083 | 6704 | 0.340 |
| 2 | 11.872 | 29414 | 6014 | 0.277 |
| 3 | 12.087 | 122227 | 24487 | 1.151 |
| 4 | 12.307 | 59541 | 12693 | 0.561 |
| 5 | 12.538 | 10088536 | 1340250 | 95.016 |
| 6 | 12.880 | 281927 | 53186 | 2.655 |
| Total | | 10617728 | 1443333 | 100.000 |