


Sample Name : Proctolin  
Cat. No. : RP10475

Pump A : 0.065% trifluoroacetic in 100% water  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
Total Flow : 1 ml / min  
Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<Detector A>  
Column : SHIMADZU VP-ODS 4.6 x 150 mm

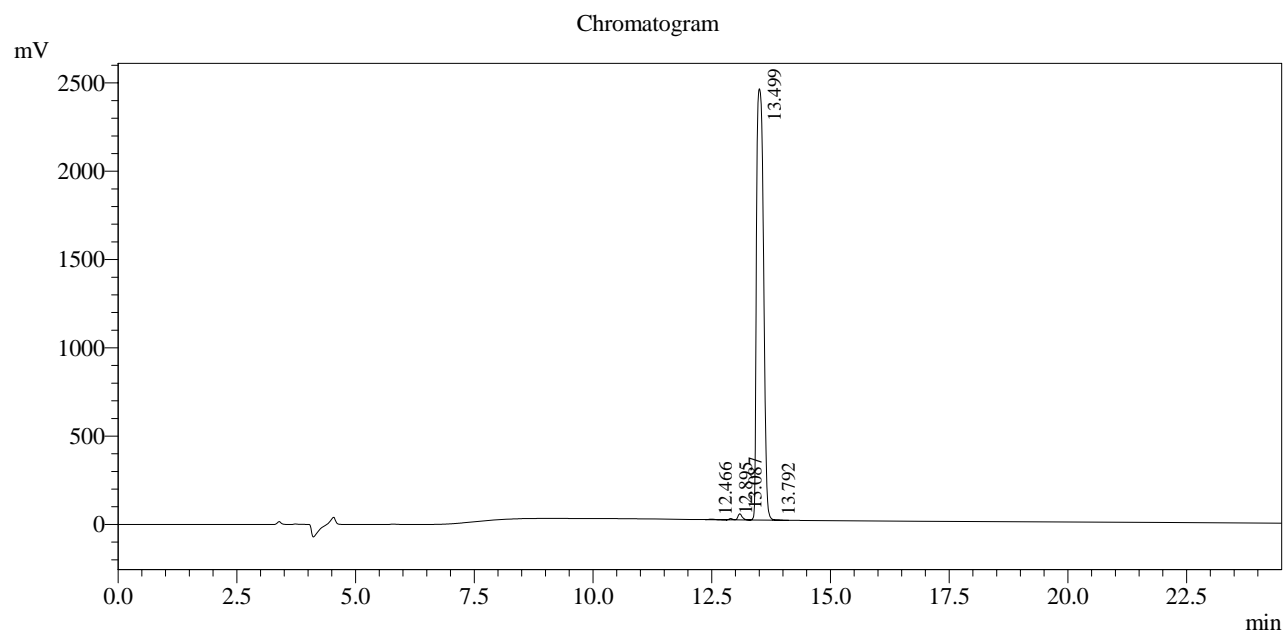

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	12.466	23002	2059	0.091
2	12.895	37665	7396	0.149
3	13.087	212003	35028	0.840
4	13.499	24939819	2442256	98.853
5	13.792	16589	4005	0.066
Total		25229077	2490745	100.000