


Sample Name : Motilin,human,porcine  
Cat. No. : RP10527

Pump A : 0.065% trifluoroacetic in 100% water  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
Total Flow : 1 ml / min  
Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>  
Column : SHIMADZU VP-ODS 4.6 x 150 mm

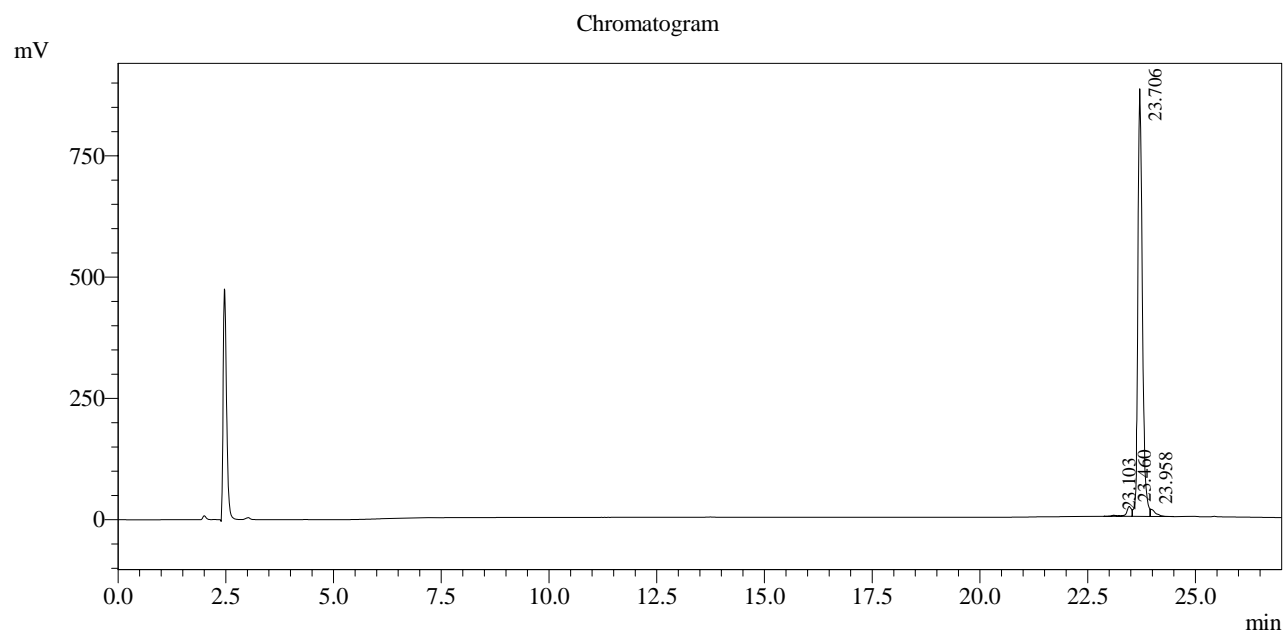

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	23.103	19477	2240	0.289
2	23.460	154239	20444	2.285
3	23.706	6453712	881481	95.616
4	23.958	122200	14821	1.810
Total		6749629	918986	100.000