

Sample Name : CRF,human,rat  
Cat. No. :RP10982  
Lot. No. :CD07908

Pump A : 0.065% trifluoroacetic in 100% water  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
Total Flow:1 ml/min  
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

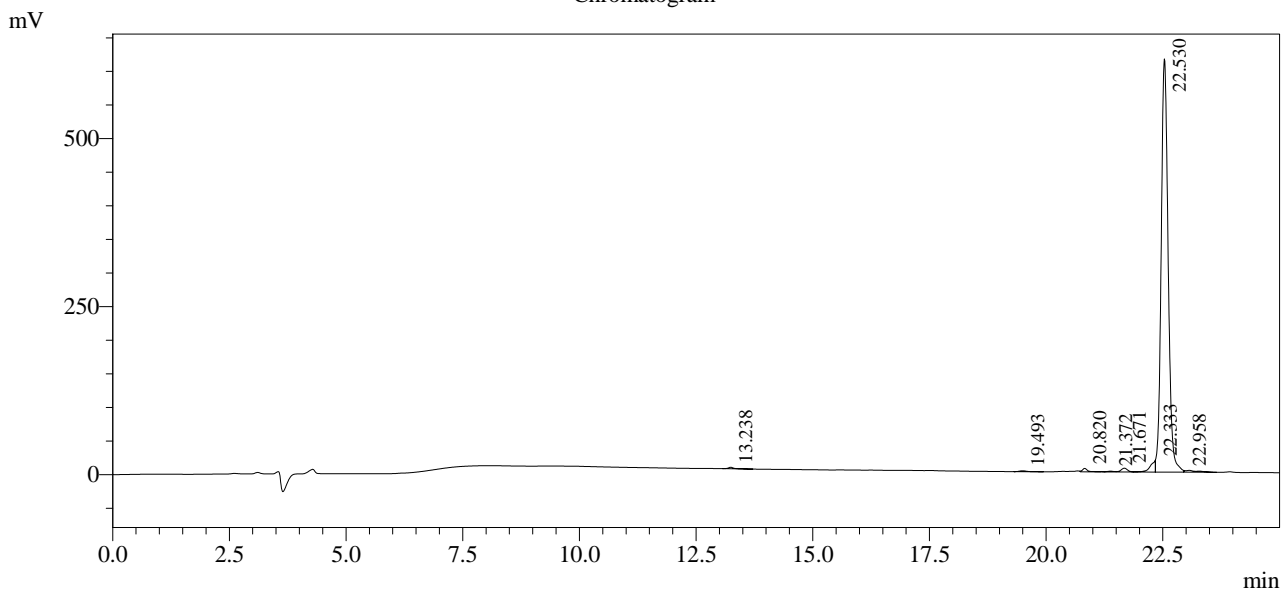

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.238	18067	2214	0.270
2	19.493	14108	1310	0.211
3	20.820	44849	5161	0.670
4	21.372	12486	1134	0.186
5	21.671	55388	5689	0.827
6	22.333	131597	16684	1.965
7	22.530	6377206	614929	95.222
8	22.958	43487	2401	0.649
Total		6697187	649522	100.000