

Sample Name : Bombesin
Cat. No. :RP11157
Lot. No. :CD03905

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

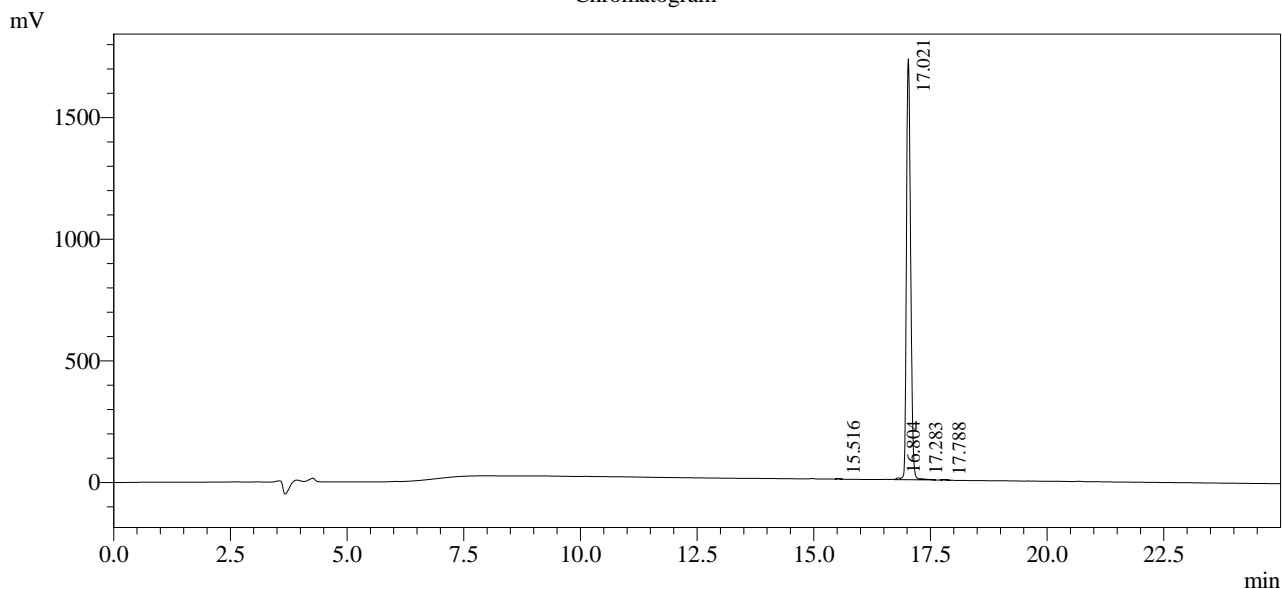

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.516	11696	2600	0.108
2	16.804	39844	7223	0.367
3	17.021	10762648	1729786	99.015
4	17.283	43188	3770	0.397
5	17.788	12359	1997	0.114
Total		10869735	1745376	100.000