

Sample Name : Angiotensin II,human  
Cat. No. :RP11257  
Lot. No. :CD16907

Pump A : 0.065% trifluoroacetic in 100% water  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
Total Flow:1 ml/min  
Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

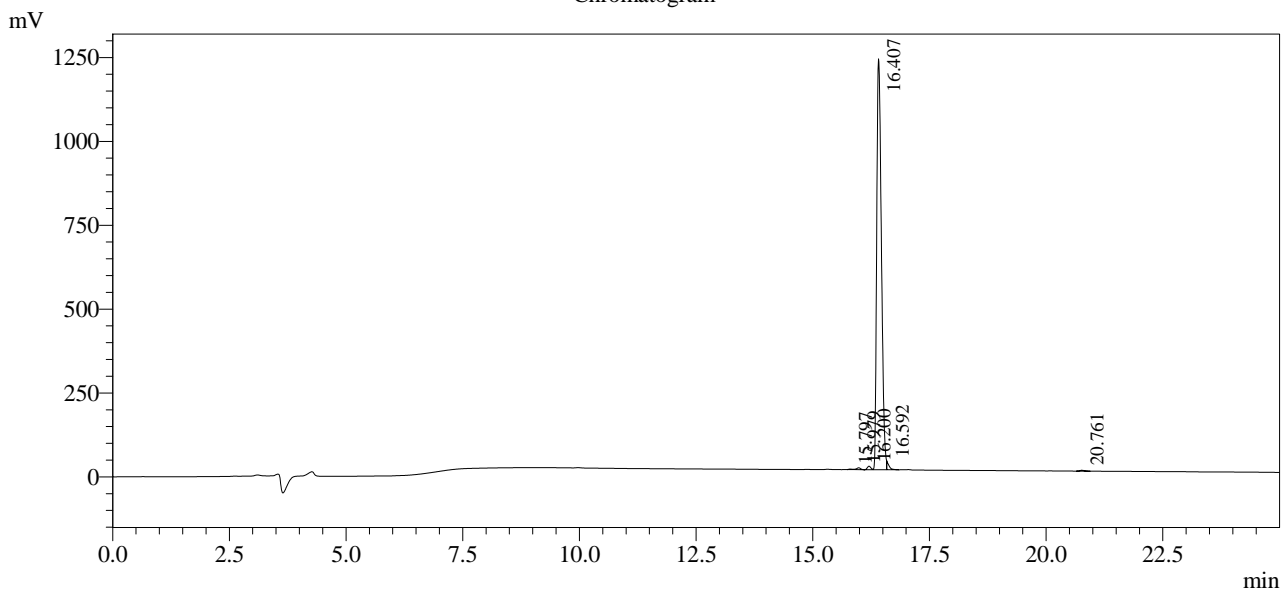

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.797	9065	1551	0.104
2	15.979	32964	5518	0.377
3	16.200	55639	10464	0.636
4	16.407	8561688	1224801	97.797
5	16.592	79394	23287	0.907
6	20.761	15768	2553	0.180
Total		8754518	1268174	100.000