

Sample Name : HA peptide
Cat. No. :RP11735
Lot. No. :CA16907

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

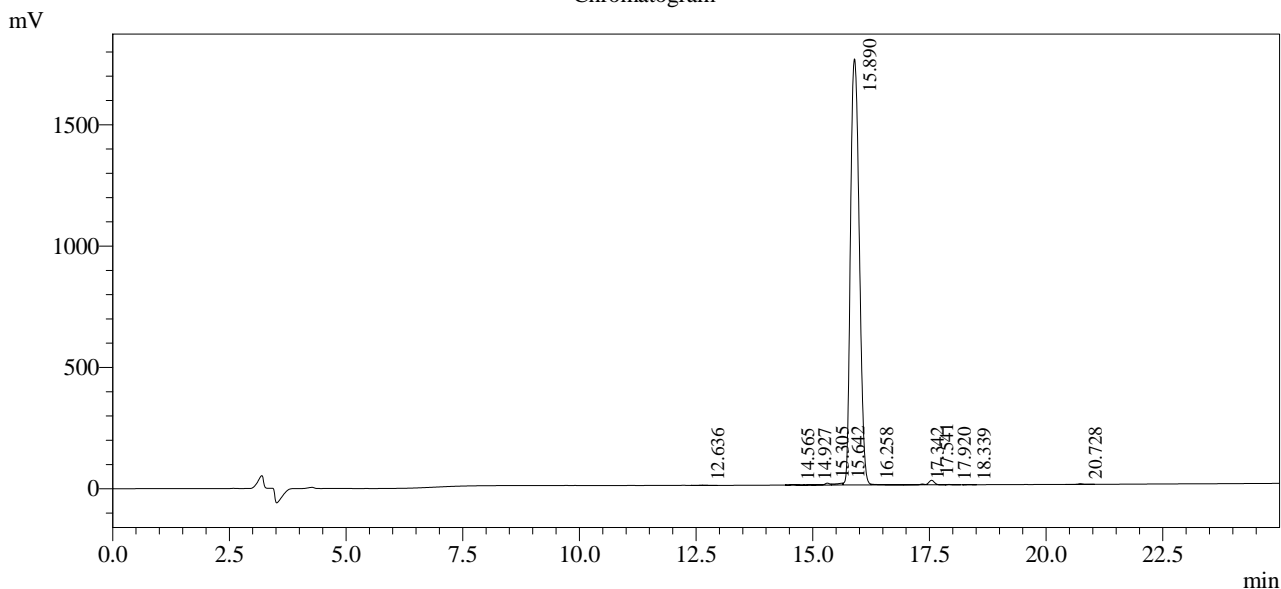

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.636	9514	1021	0.040
2	14.565	18478	2259	0.078
3	14.927	8538	1339	0.036
4	15.305	68878	7980	0.292
5	15.642	83940	7962	0.356
6	15.890	23134130	1755979	98.163
7	16.258	44415	3211	0.188
8	17.342	23410	3325	0.099
9	17.541	152513	18711	0.647
10	17.920	7228	1415	0.031
11	18.339	2590	313	0.011
12	20.728	13535	2198	0.057
Total		23567169	1805714	100.000