


Sample Description:

Structure : LS-37
 Column : 4.6×250mm, Sinochrom ODS-BP-5
 Solvent A : 0.05% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.065% trifluoroacetic in 100% water
 Gradient :
 A B
 0.01min 42% 58%
 25min 52% 48%
 25.1min 100% 0%
 30min STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

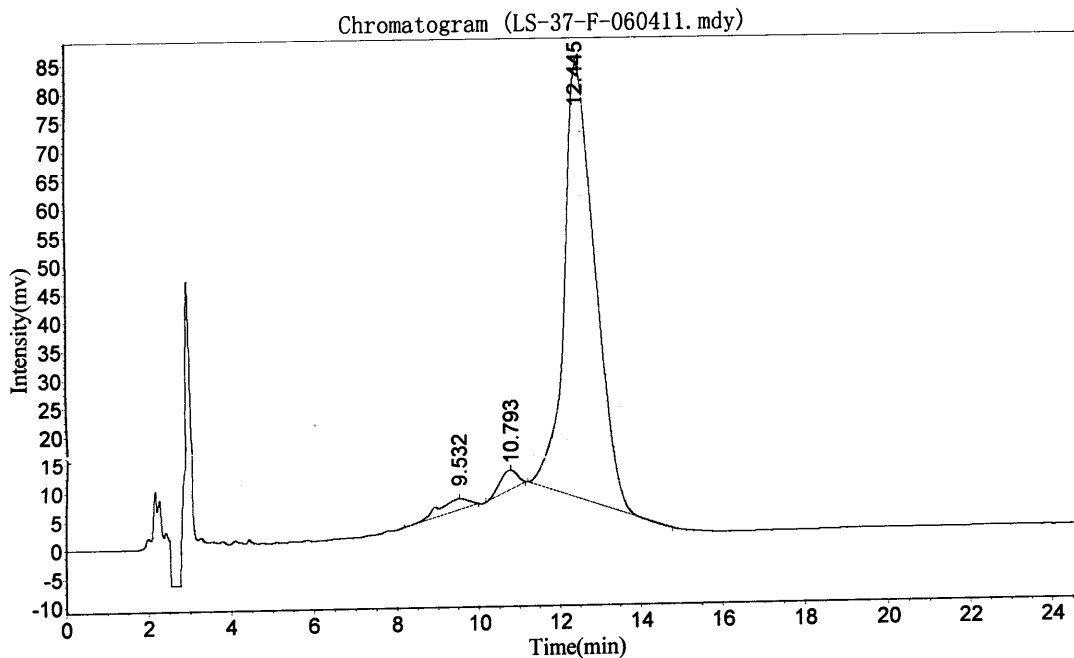

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		9.532	1900.312	107367.938	2.5076
2		10.793	3434.374	104955.289	2.4512
3		12.445	76457.180	4069458.750	95.0412
Total			81791.865	4281781.977	100.0000