


Sample Name : Flu-M1  
Cat. No. : RP19978

Pump A : 0.065% trifluoroacetic in 100% water  
Pump A : 0.05% trifluoroacetic in 100% acetonitrile  
TotalFlow:1 ml/min  
Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>  
Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

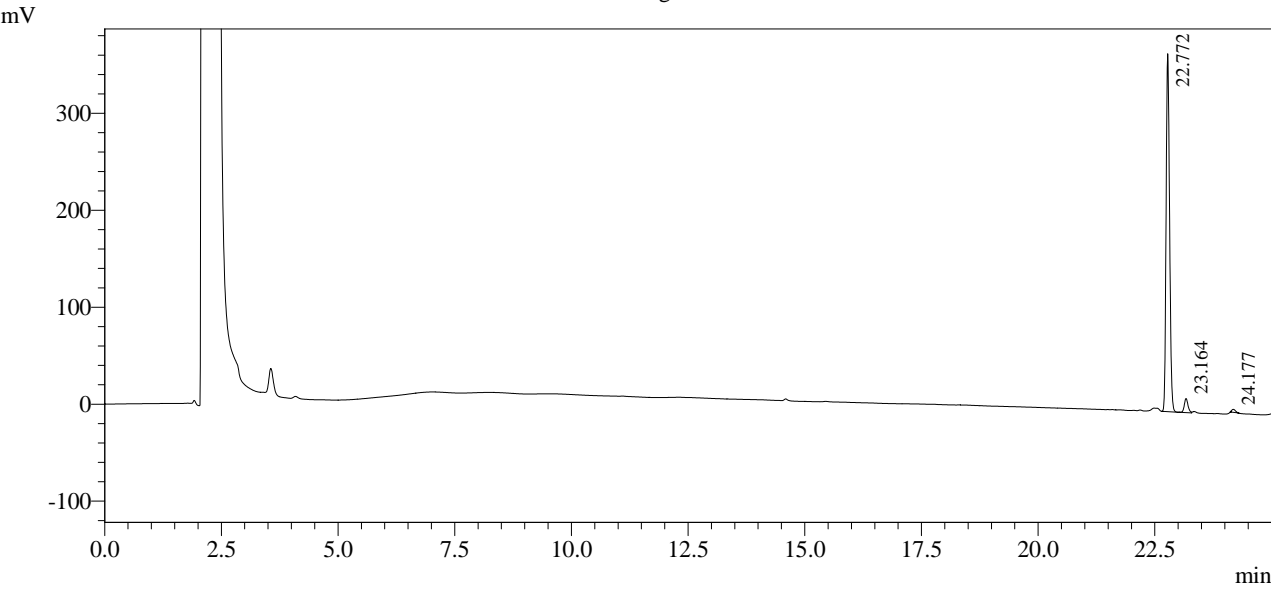

1 Det.A Ch1 / 214nm

Peak Table

Peak#	Ret. Time	Area	Height	Area %
1	22.772	1910334	369180	95.158
2	23.164	80335	14555	4.002
3	24.177	16865	3048	0.840
Total		2007534	386784	100.000