


Sample Name : NY-BR-1 p904 (A2)
Cat No. : RP19987

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
TotalFlow : 1 ml / min
Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

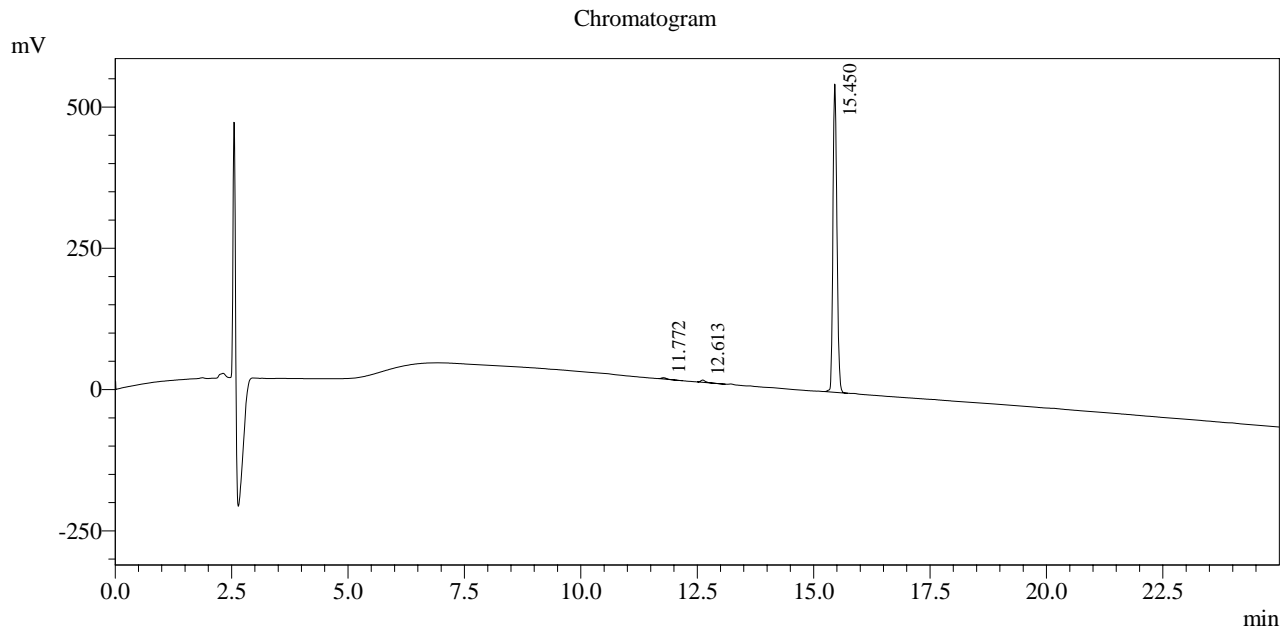

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	11.772	18643	2422	0.568
2	12.613	28735	4011	0.875
3	15.450	3236420	545566	98.557
Total		3283798	551999	100.000