


Sample Name : LSKL, Inhibitor of Thrombospondin (TSP-1)
Cat No. : RP19990

Pump A : 0.065% trifluoroacetic in 100% water
Pump A : 0.05% trifluoroacetic in 100% acetonitrile
TotalFlow:1 ml/min
Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

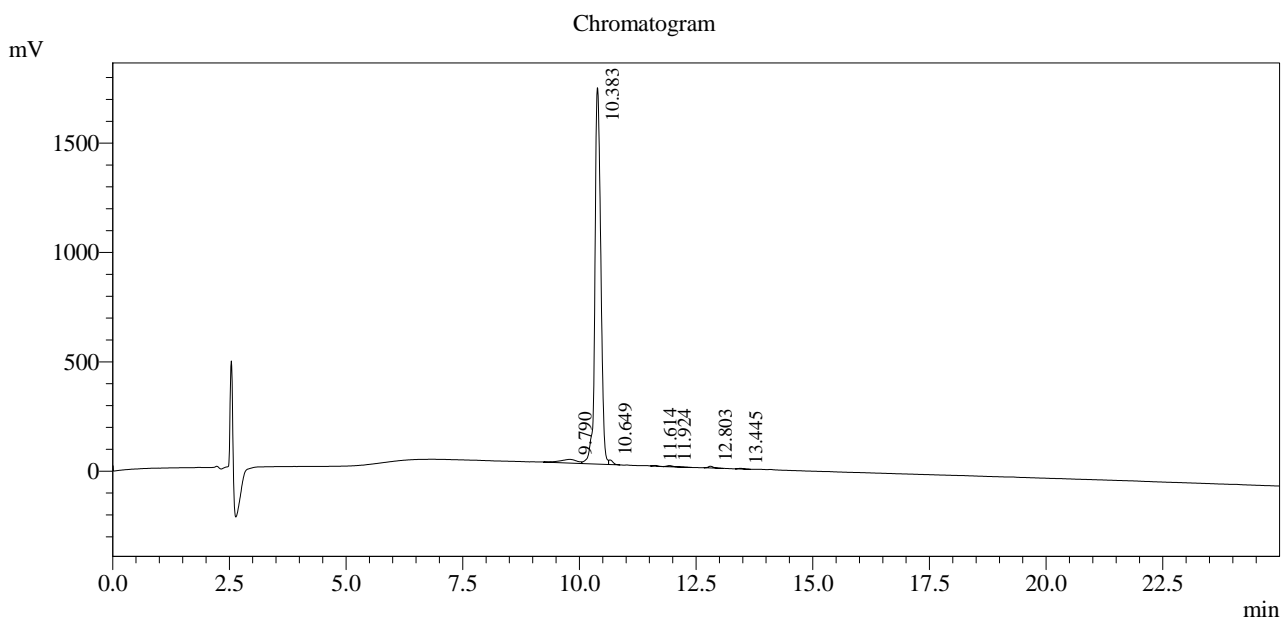

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	9.790	408674	16513	2.585
2	10.383	15121004	1721152	95.649
3	10.649	123189	20710	0.779
4	11.614	17382	2968	0.110
5	11.924	54855	5161	0.347
6	12.803	61070	8022	0.386
7	13.445	22632	3107	0.143
Total		15808805	1777631	100.000