


Positive

MS Spectrum

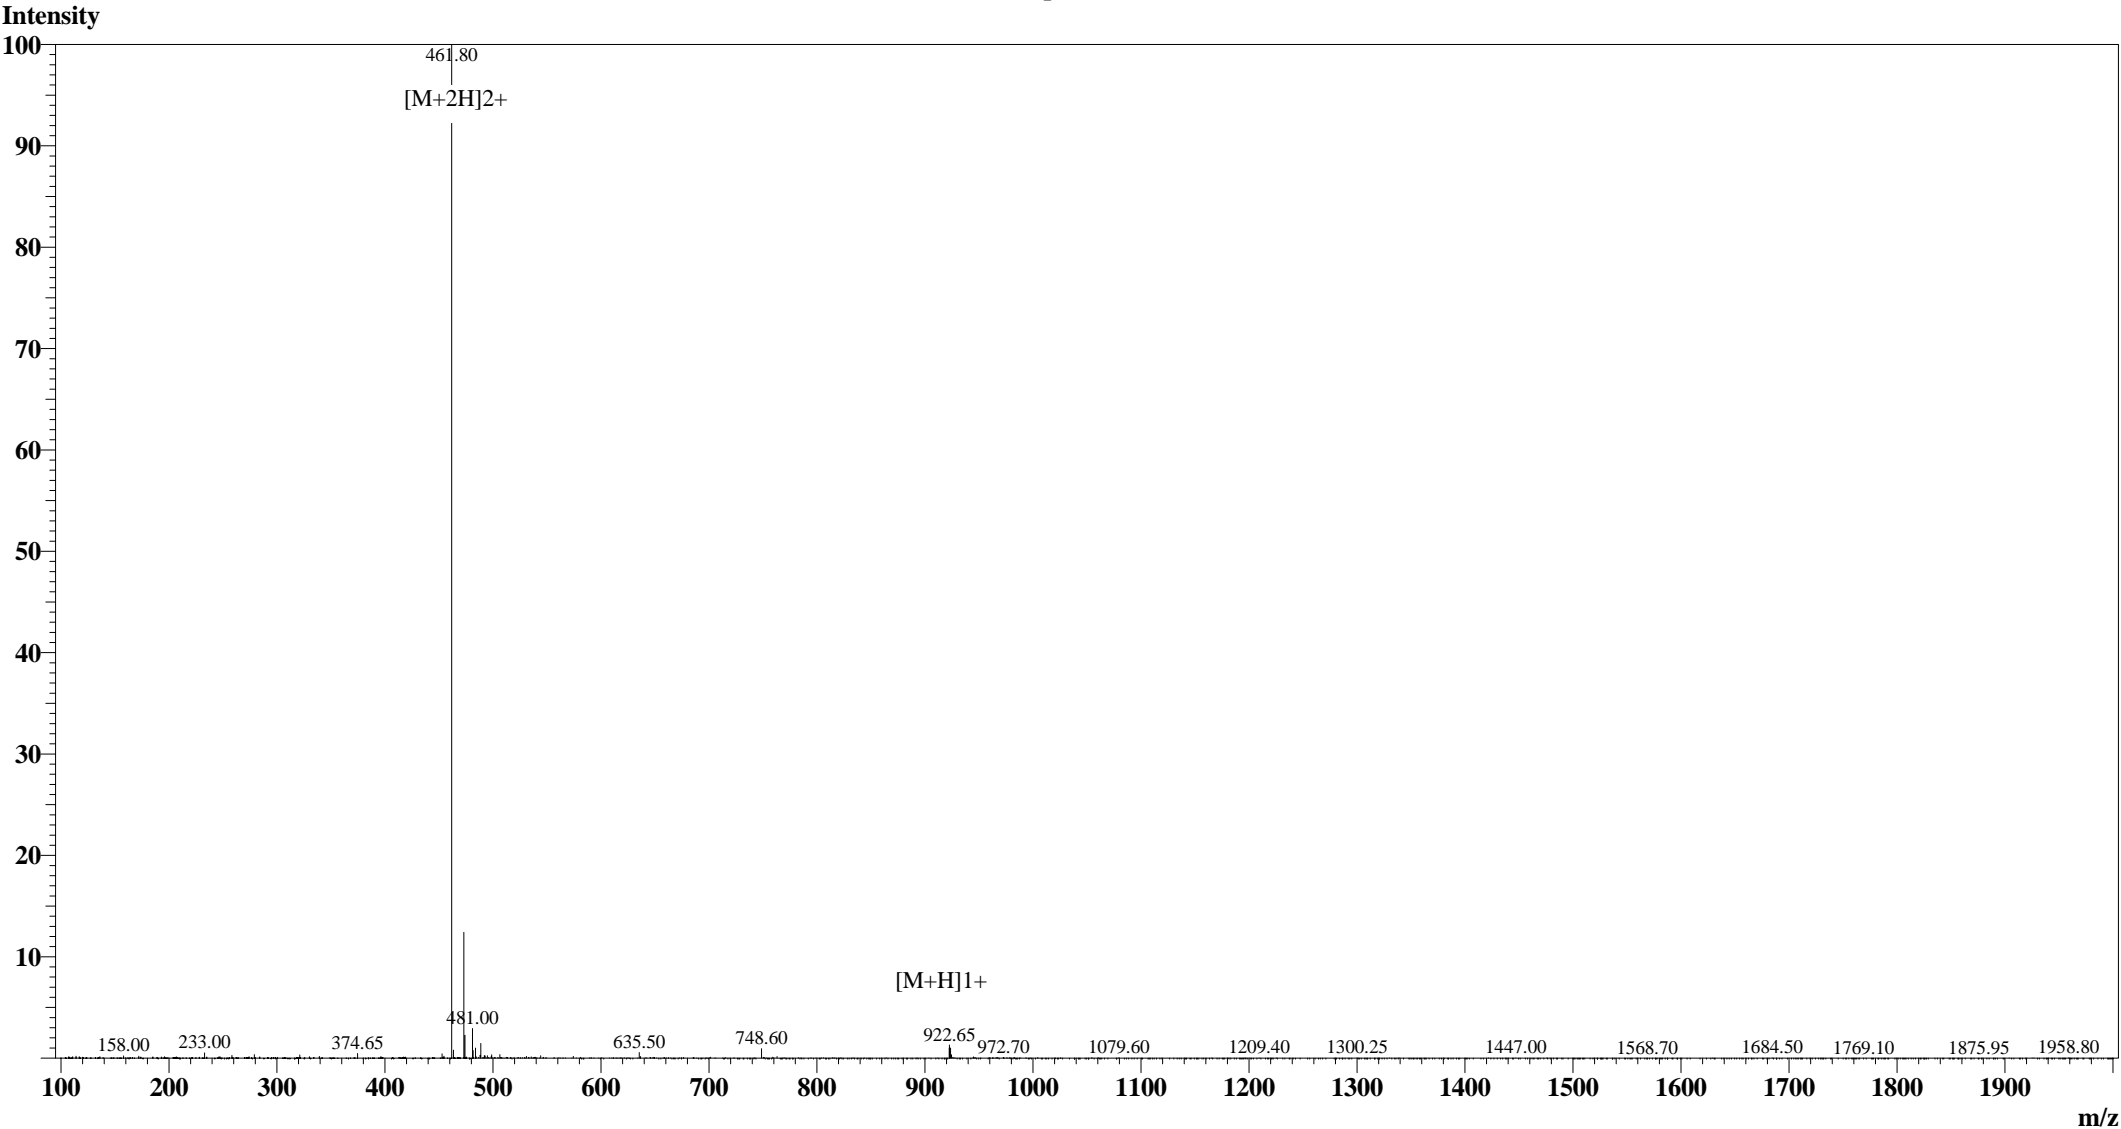

Sample Information		Interface		Prerod Bias	
User	:xu	Nebulizing Gas Flow	:ESI	Detector	:+4.5kv
Date Acquired	: 2008-4-23 14:42:02	CDL Temp	:1.50 L/min	T.Flow	:1.5kv
Sample Name	:HSV-gB2(498-505)	CDL Volt	: 250°C	B.conc	: 0.2ml/min
Cat No.	: RP19992	Block Temp	: -25.0V		: 50%H2O/50%MeOH
Injection Volum	: 1.000μL		: 200°C		
Theoretical MW	:921.07				
Observed MW	:921.65				