


Positive

MS Spectrum

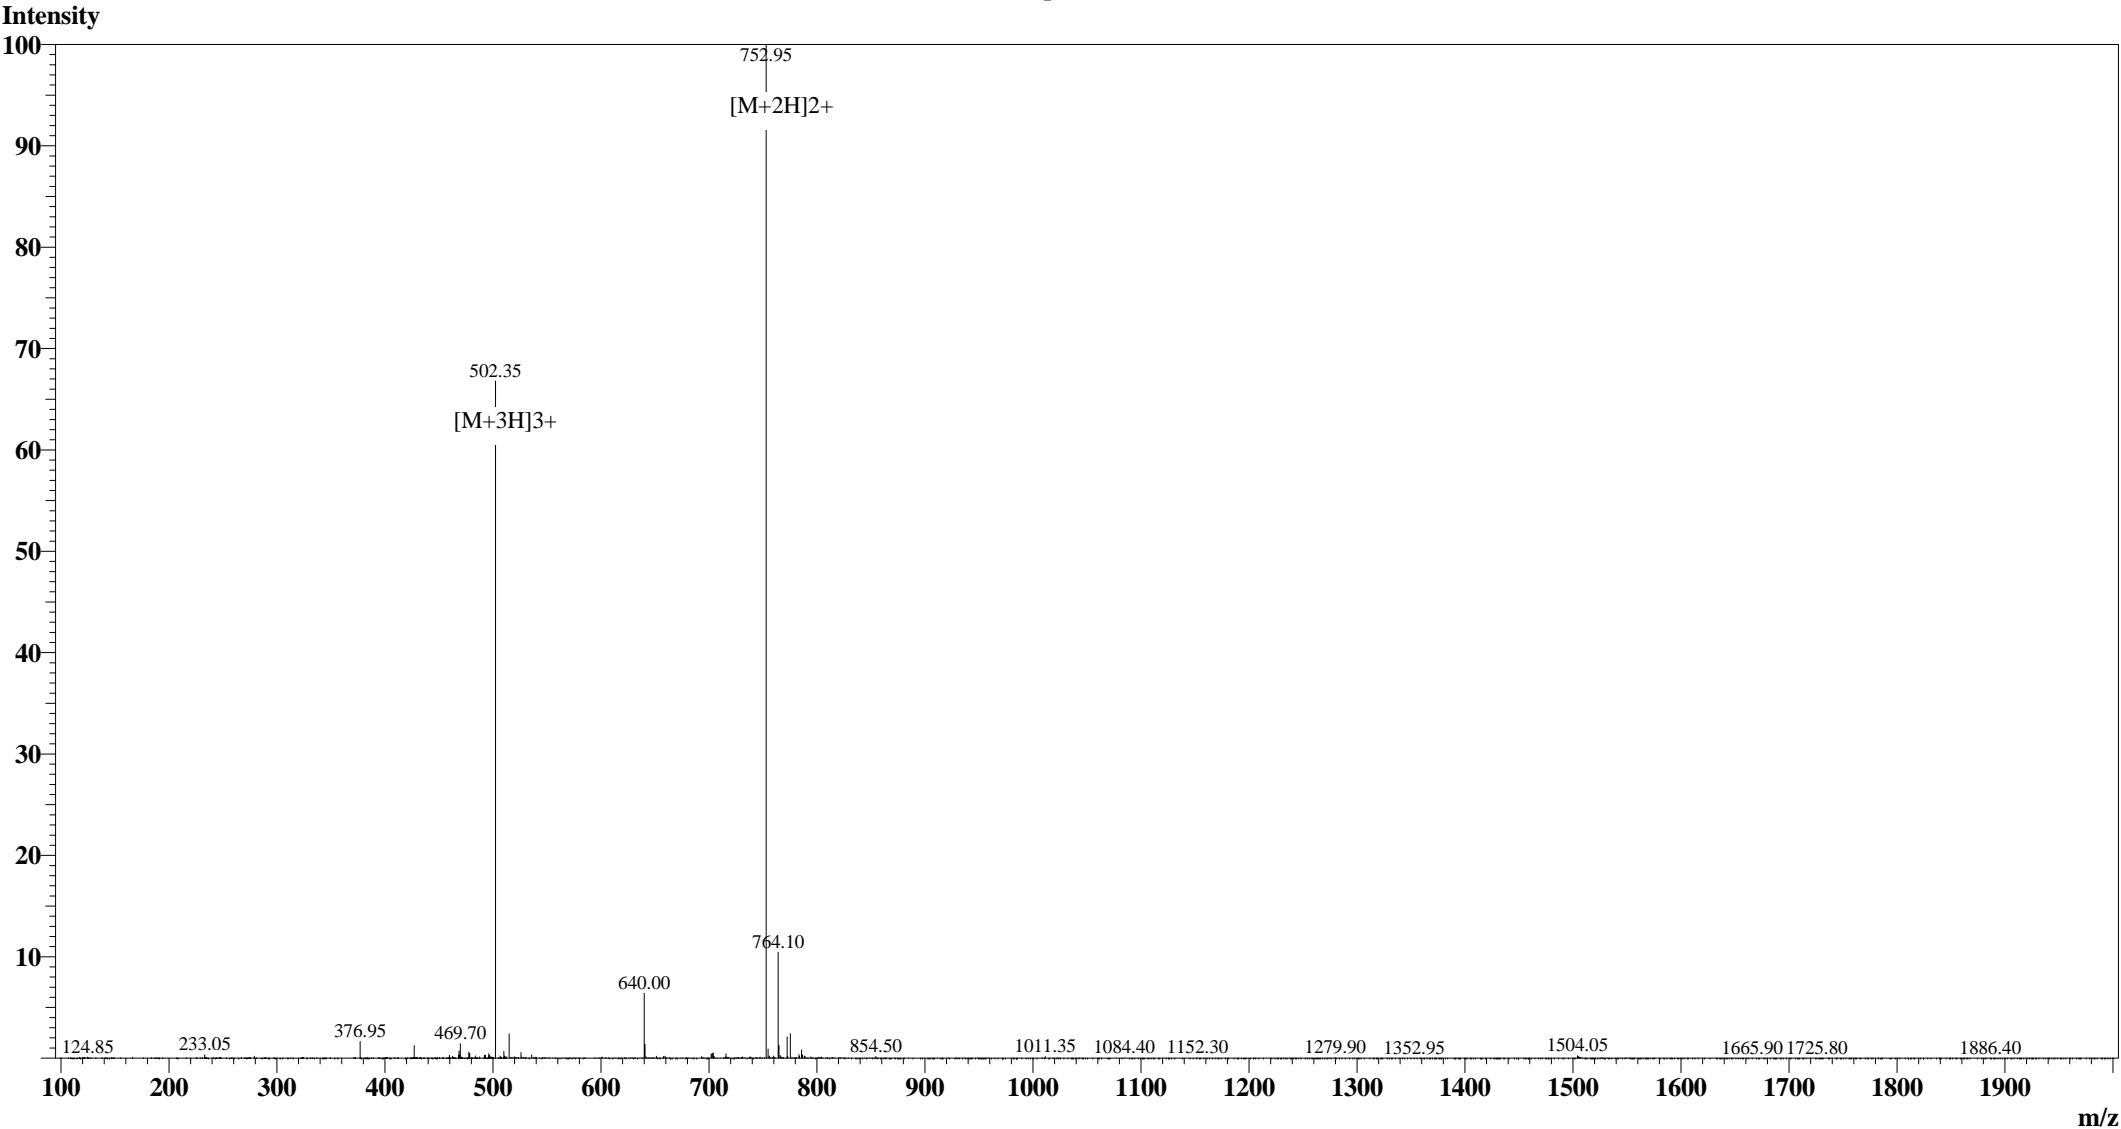

Sample Information		Interface		Prerod Bias	
User	:xu	Nebulizing Gas Flow	:1.50 L/min	Detector	:1.5kv
Date Acquired	: 2008-4-18 9:13:50	CDL Temp	: 250°C	T.Flow	: 0.2ml/min
Sample Name	:Influenza Hemagglutinin(307-319)	CDL Volt	: -25.0V	B.conc	: 50%H2O/50%MeOH
Cat No.	: RP20087	Block Temp	: 200°C		
Injection Volum	: 1.000µL				
Theoretical MW	:1503.82				
Observed MW	:1503.90				