

Sample Name : TAT 2-4
Cat No. : RP10131


Pump A : 0.065% trifluoroacetic in 100% water
Pump A : 0.05% trifluoroacetic in 100% acetonitrile
TotalFlow:1 ml/min
Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

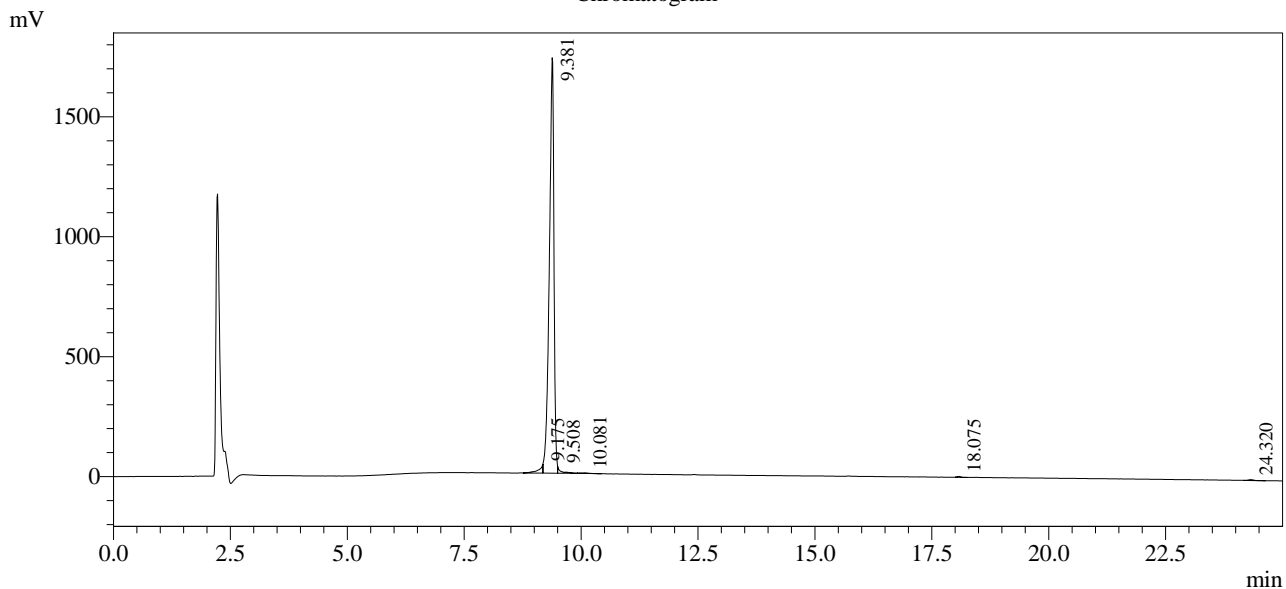

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	9.175	226375	32373	1.840
2	9.381	11900109	1731739	96.716
3	9.508	106250	22361	0.864
4	10.081	24401	1908	0.198
5	18.075	18386	3882	0.149
6	24.320	28621	3406	0.233
Total		12304142	1795670	100.000