

Sample Name : Neurotensin
Cat. No. :RP10439
Lot. No. :CD17907

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

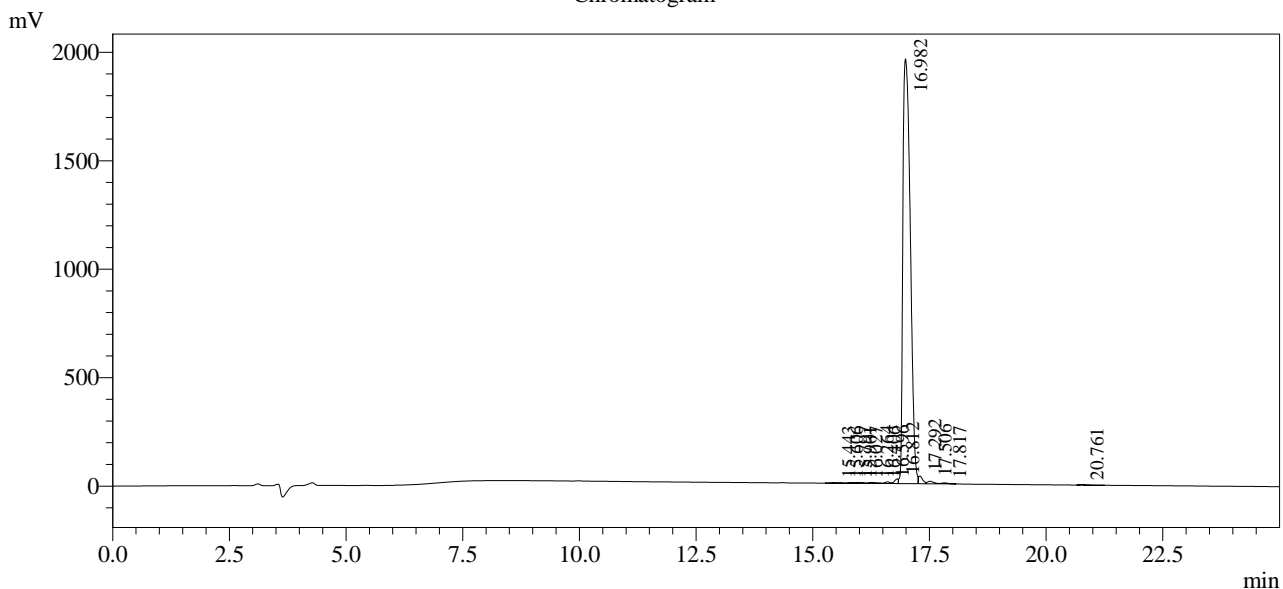

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.443	14841	1915	0.066
2	15.606	12672	1976	0.056
3	15.797	21676	2840	0.097
4	15.901	19885	3198	0.089
5	16.027	31454	4070	0.140
6	16.264	42545	4589	0.190
7	16.406	19751	2941	0.088
8	16.596	57929	7847	0.258
9	16.812	117334	20990	0.523
10	16.982	21716170	1958335	96.769
11	17.292	214378	34993	0.955
12	17.506	110181	11672	0.491
13	17.817	45454	4672	0.203
14	20.761	17044	2585	0.076
Total		22441316	2062625	100.000