


Sample Description:
 Structure : IL-14
 Column : 4.6×250mm, Kromasil C18
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :
 A B
 0.01min 33% 67%
 25min 55% 45%
 25.1min 100% 0%
 30min STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

RP10465
 PY00809508

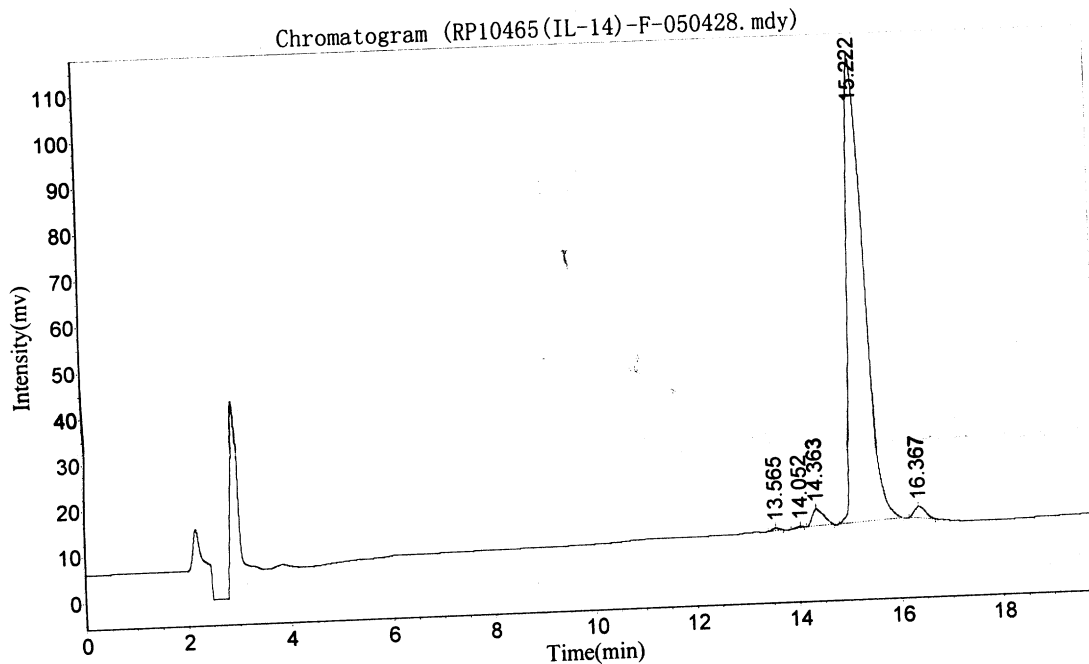

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		13.565	571.858	5537.801	0.2314
2		14.052	228.590	2241.998	0.0937
3		14.363	3701.455	57172.789	2.3888
4		15.222	101088.523	2289036.500	95.6423
5		16.367	2573.351	39342.168	1.6438
Total			108163.777	2393331.256	100.0000