

Sample Name : Dermorphin
Cat. No. : RP10427
Lot. No. : CC07902


Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow : 1 ml / min
Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
35.00	Pumps	Pump B Conc.	95	
35.01	Pumps	Pump B Conc.	5	
43.00	Pumps	Pump B Conc.	5	
43.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Atlantis T3 4.6 x 250 mm

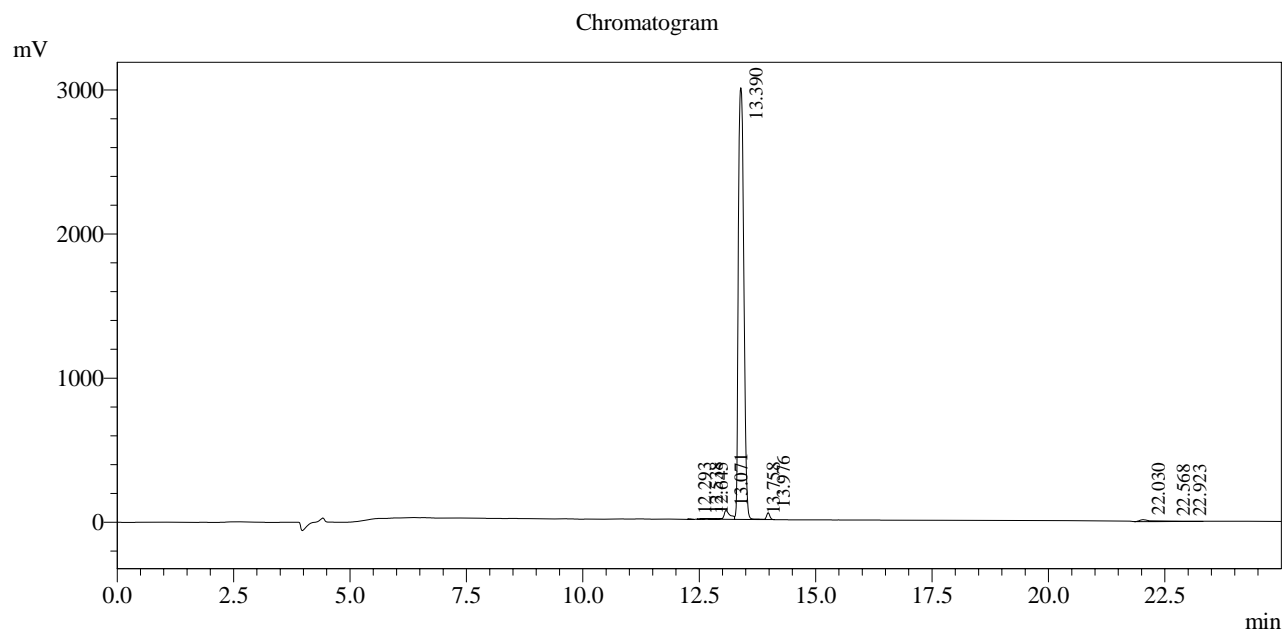

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	12.293	6112	1548	0.024
2	12.538	15934	3076	0.062
3	12.645	61926	4309	0.241
4	13.071	573658	61579	2.231
5	13.390	24443313	2995660	95.075
6	13.758	17781	3449	0.069
7	13.976	226492	47470	0.881
8	22.030	173530	12827	0.675
9	22.568	85941	3547	0.334
10	22.923	104774	3253	0.408
Total		25709461	3136716	100.000