

Sample Name : ACTH) (1-24), human
 Cat. No. : RP11303
 Lot. No. : CB02910

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

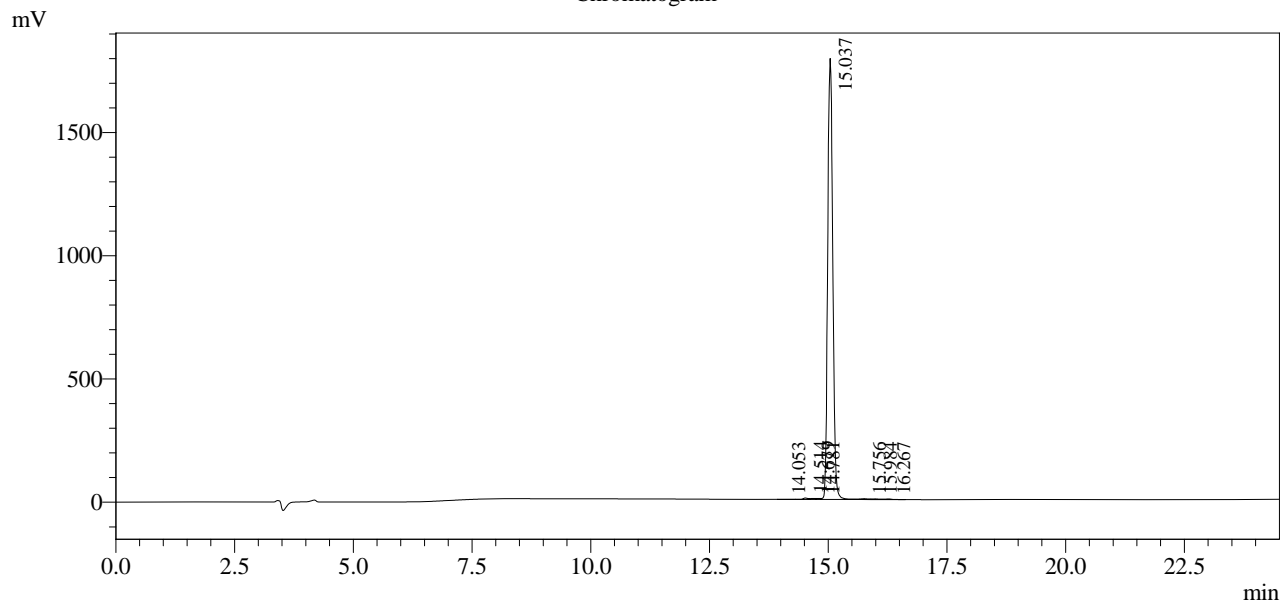

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.053	10199	1182	0.075
2	14.514	39378	5563	0.290
3	14.679	30071	4005	0.221
4	14.781	27398	4086	0.202
5	15.037	13361931	1789766	98.413
6	15.756	47486	3351	0.350
7	15.984	31084	2746	0.229
8	16.267	29875	2653	0.220
Total		13577421	1813353	100.000