


Sample Description:
 Structure : DA-29-1
 Column : 4.6×250mm, Kromasil C18-5
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :
 A B
 0.01min 30% 70%
 25min 50% 50%
 25.1min 100% 0%
 30min STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

RP10341
 PX00409508

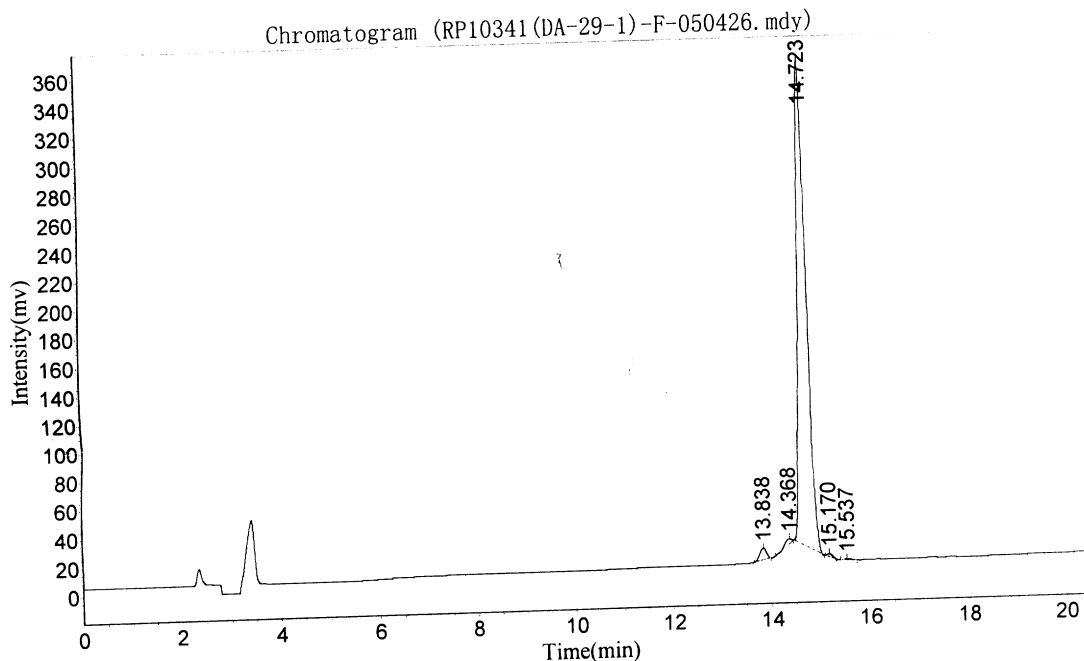

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		13.838	8177.130	78351.805	1.8006
2		14.368	3672.816	33756.102	0.7758
3		14.723	339324.313	4213983.500	96.8418
4		15.170	2246.430	16874.506	0.3878
5		15.537	875.032	8442.407	0.1940
Total			354295.721	4351408.319	100.0000