


Positive

Intensity

MS Spectrum

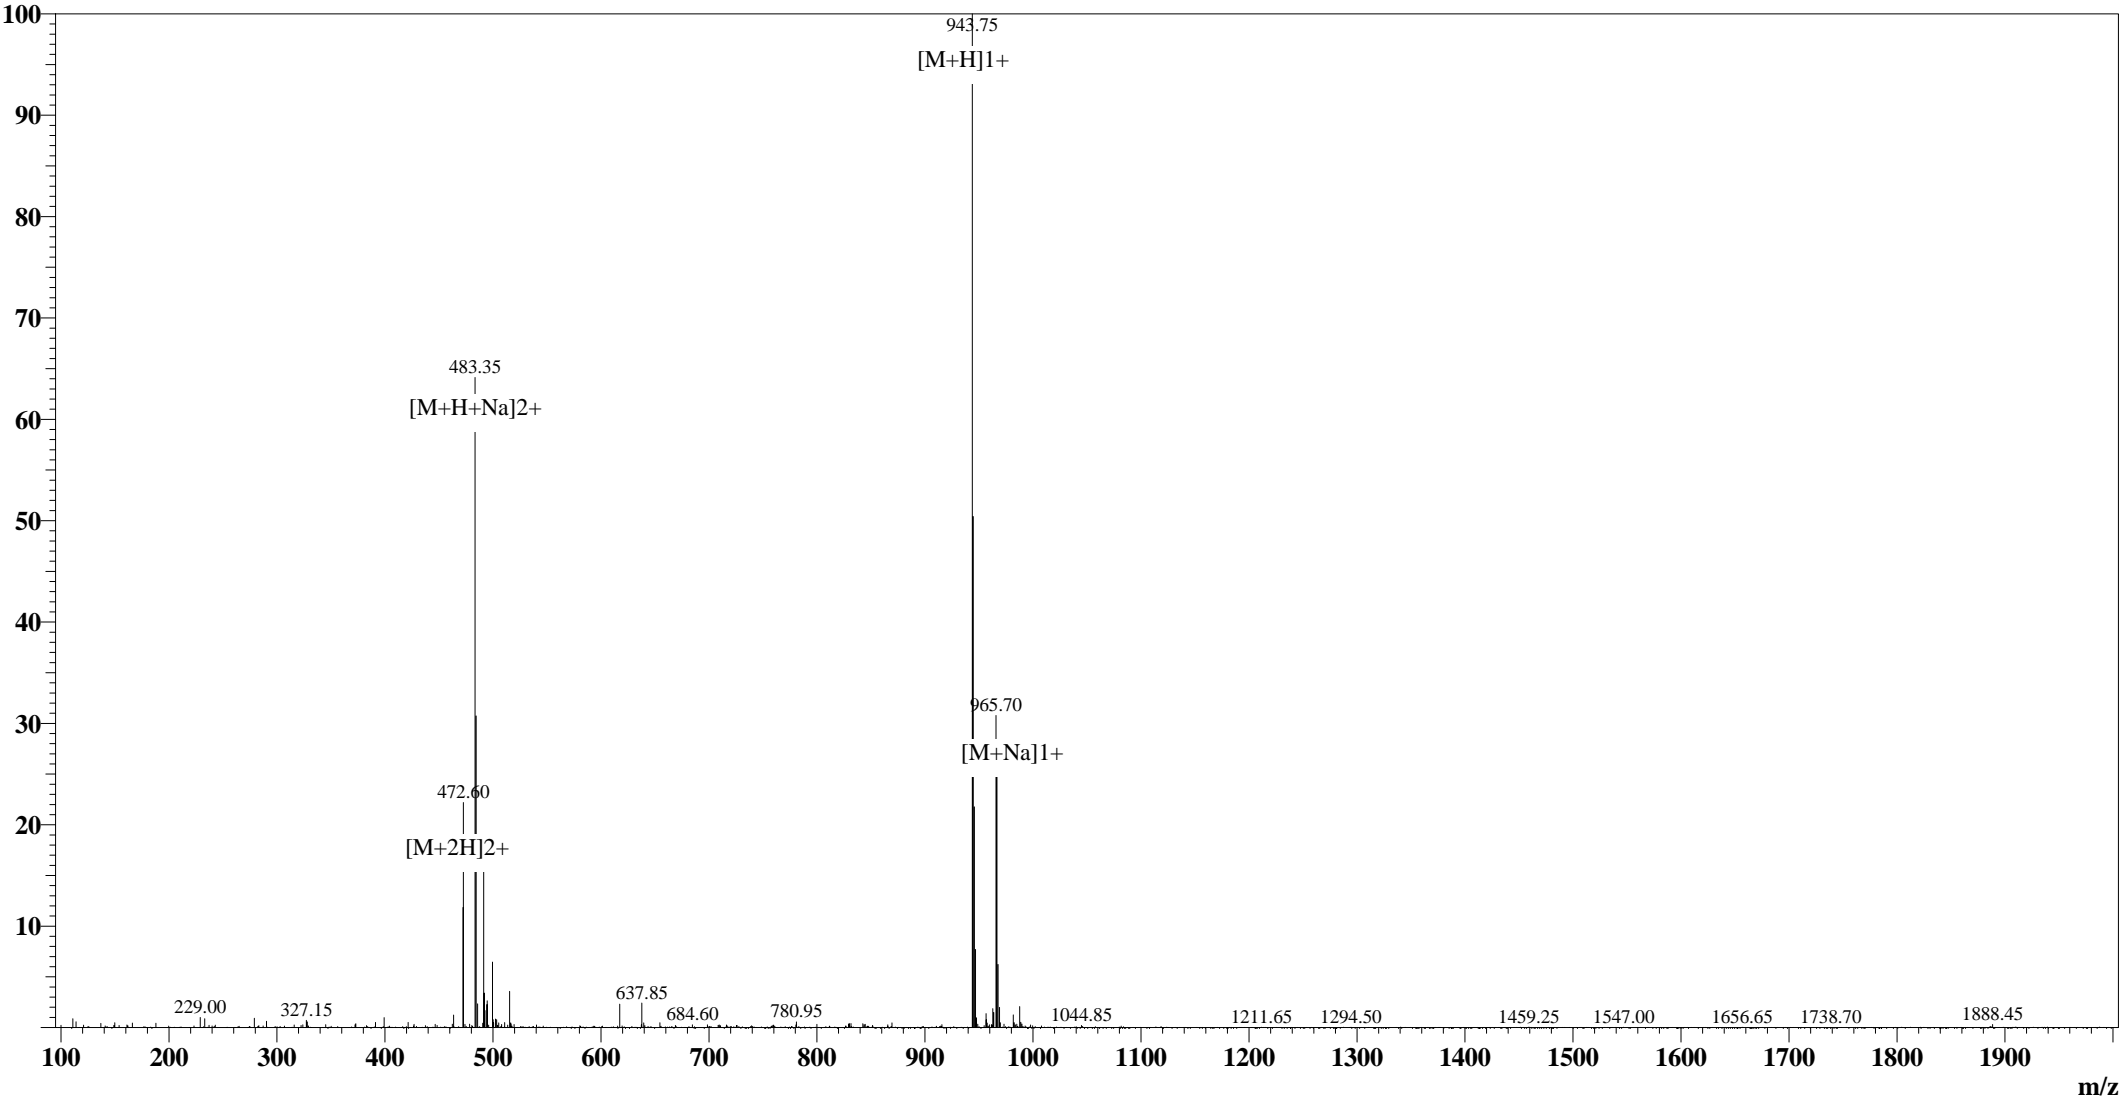

Sample Information

User :xu  
Date Acquired : 2008-4-18 9:05:47  
Sample Name :CEF20  
Cat No. :RP11781  
Injection Volum : 1.000μL  
Theoretical MW :943.18  
Observed MW :942.75

Interface :ESI  
Nebulizing Gas Flow :1.50 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias :+4.5kv  
Detector :1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH