

Sample Name : Beta-Amyloid (1-15)
 Cat. No. : RP20141
 Lot. No. : CA04902


Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : X Bridge 4.6 x 250mm

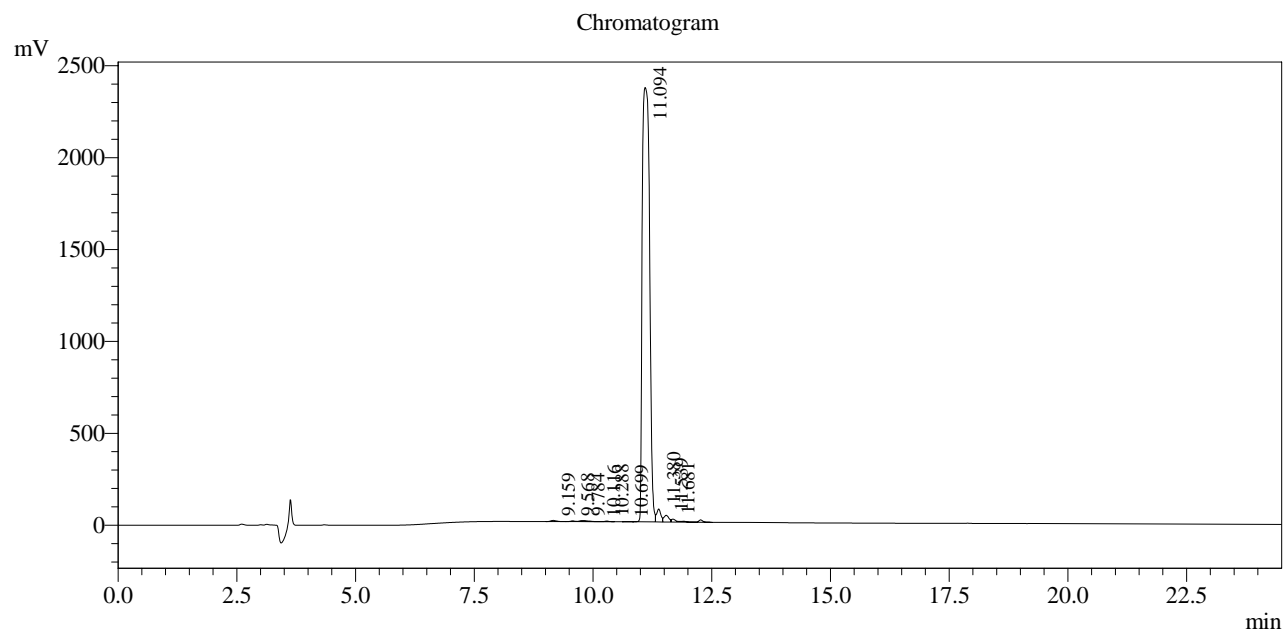

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	9.159	52850	6660	0.200
2	9.568	26287	4308	0.099
3	9.784	77376	5960	0.293
4	10.116	5431	841	0.021
5	10.288	17156	3242	0.065
6	10.699	2422	451	0.009
7	11.094	25333356	2364003	95.854
8	11.380	428619	70714	1.622
9	11.539	269047	36629	1.018
10	11.681	216701	16002	0.820
Total		26429244	2508809	100.000