

Sample Name : Beta-Amyloid (1-17)
Cat. No. :RP20161
Lot. No. :CA06902

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

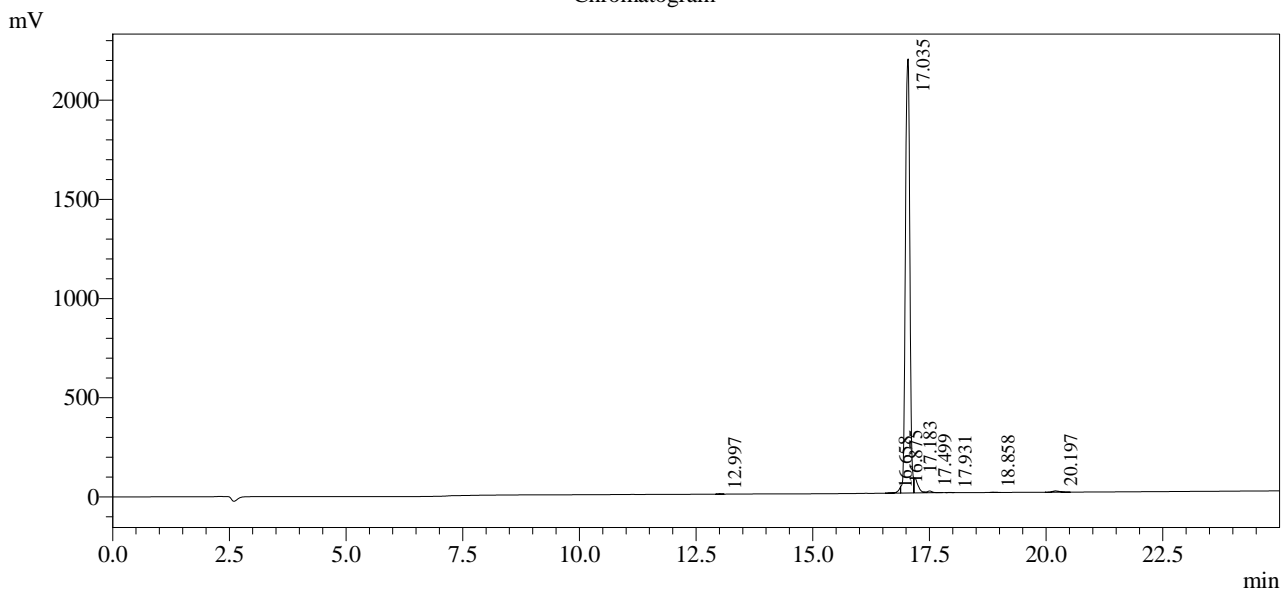

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	12.997	5042	984	0.033
2	16.658	9855	1385	0.065
3	16.875	102279	28519	0.672
4	17.035	14530342	2188210	95.403
5	17.183	440463	75254	2.892
6	17.499	62312	8854	0.409
7	17.931	4987	1175	0.033
8	18.858	7440	1237	0.049
9	20.197	67701	6429	0.445
Total		15230420	2312047	100.000