


Sample Name : Beta-Amyloid(1-20)
 Cat. No. : RP20162
 Lot. No. : CD05902

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

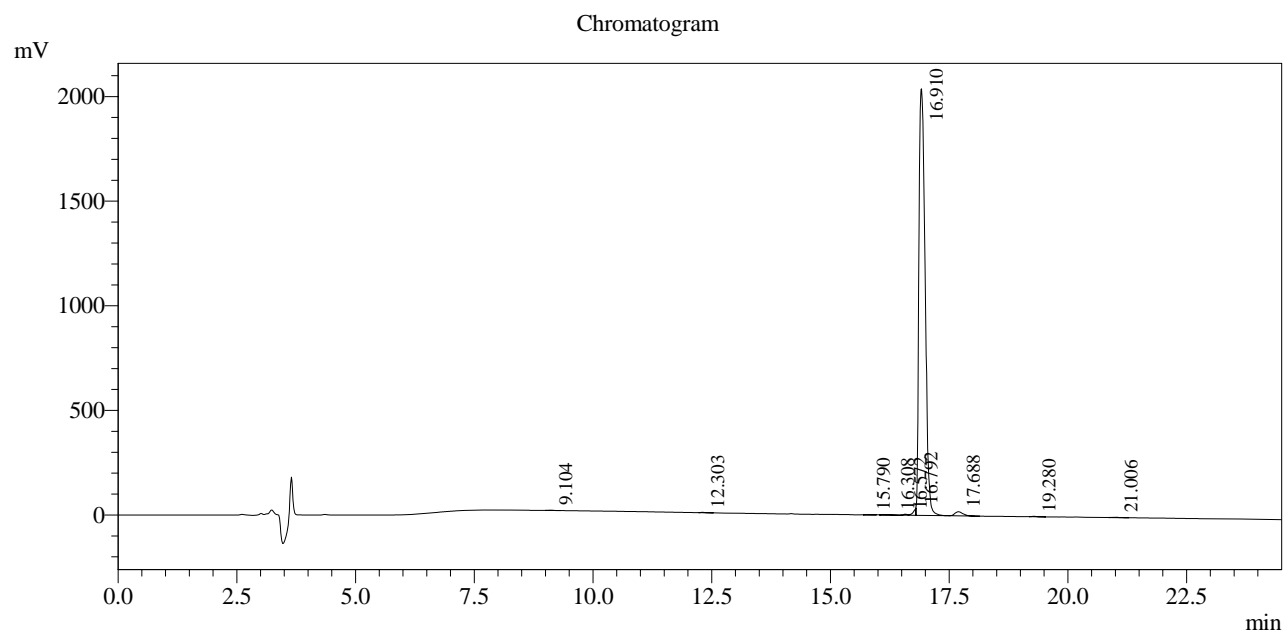

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	9.104	11190	1605	0.059
2	12.303	10125	2076	0.053
3	15.790	11447	2024	0.060
4	16.308	20215	2214	0.107
5	16.572	27992	4999	0.148
6	16.792	130839	31480	0.690
7	16.910	18485676	2039396	97.471
8	17.688	236587	19815	1.247
9	19.280	14540	2280	0.077
10	21.006	16665	2456	0.088
Total		18965276	2108344	100.000