

Sample Name : Beta-Amyloid(1-34)
Cat. No. :RP20140
Lot. No. :CD01905

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

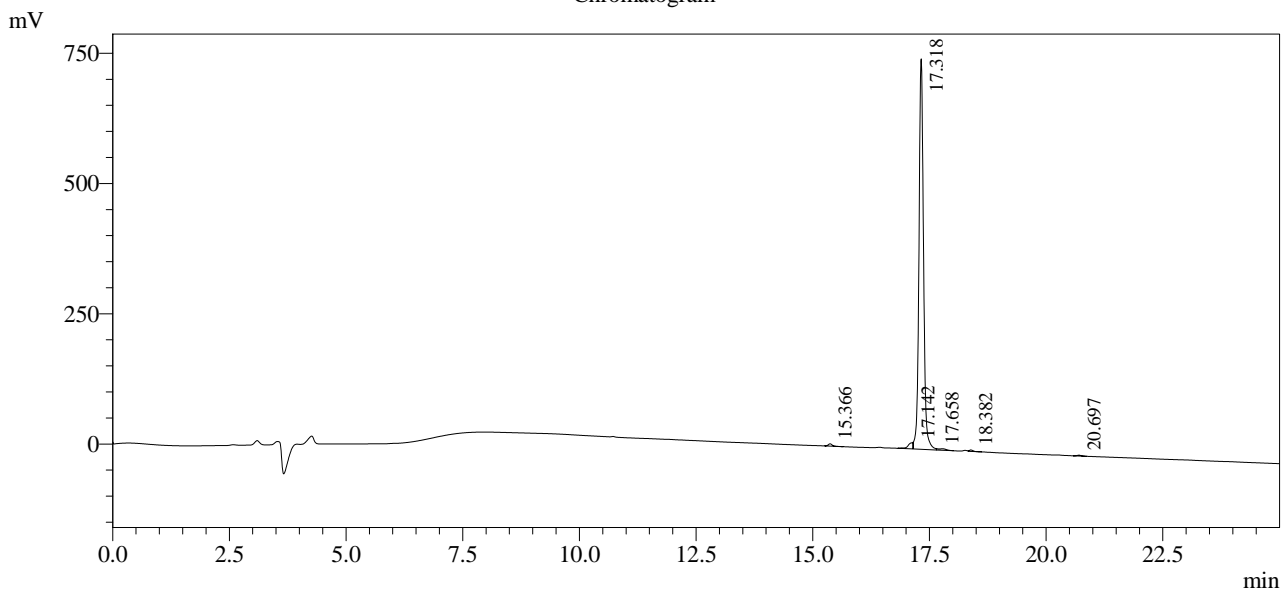

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.366	25976	4451	0.494
2	17.142	88067	12167	1.676
3	17.318	5082818	749340	96.702
4	17.658	34032	2391	0.647
5	18.382	15776	2812	0.300
6	20.697	9494	1582	0.181
Total		5256164	772743	100.000