

Sample Name : Melanotan (MT)-II  
 Cat. No. : RP17323  
 Lot. No. : CE02909

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow : 1 ml / min  
 Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

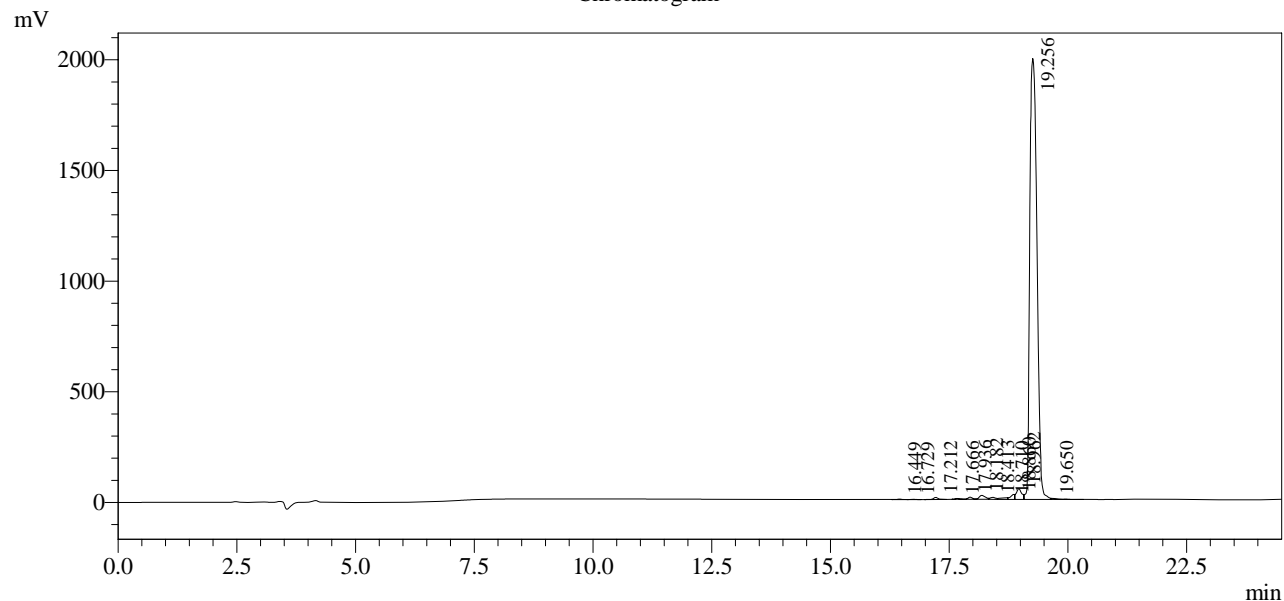

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.449	12313	2035	0.056
2	16.729	7725	1247	0.035
3	17.212	63434	9290	0.290
4	17.666	28933	3592	0.132
5	17.936	66657	9713	0.305
6	18.182	162947	17835	0.745
7	18.413	72586	9099	0.332
8	18.710	78830	7201	0.361
9	18.860	137243	22358	0.628
10	18.962	380301	47883	1.739
11	19.256	20803189	1992337	95.148
12	19.650	49829	4983	0.228
Total		21863988	2127573	100.000