

Sample Name : TLQP-30  
 Cat. No. : RP20245  
 Lot. No. : CC01906


Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow : 1 ml / min  
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

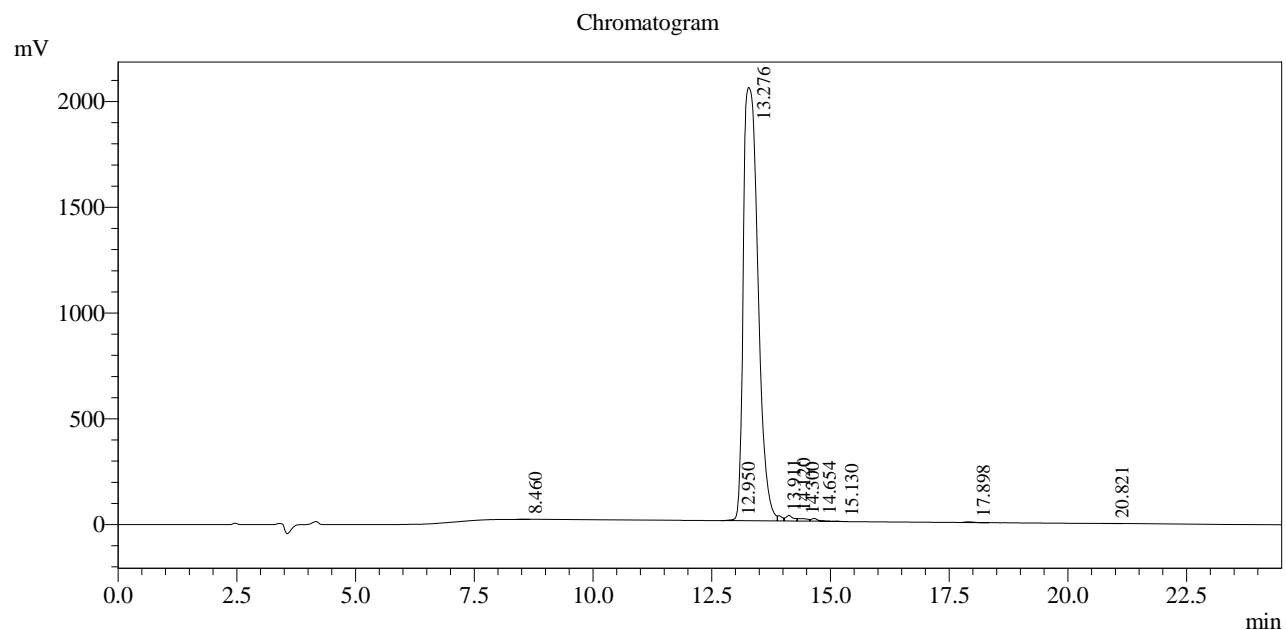

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	8.460	7104	1190	0.016
2	12.950	33272	5464	0.074
3	13.276	43992324	2048755	98.101
4	13.911	167697	24382	0.374
5	14.120	289987	26590	0.647
6	14.300	167409	11994	0.373
7	14.654	120855	13466	0.270
8	15.130	10400	1441	0.023
9	17.898	44134	3507	0.098
10	20.821	10522	1383	0.023
Total		44843704	2138172	100.000