


Positive

MS Spectrum

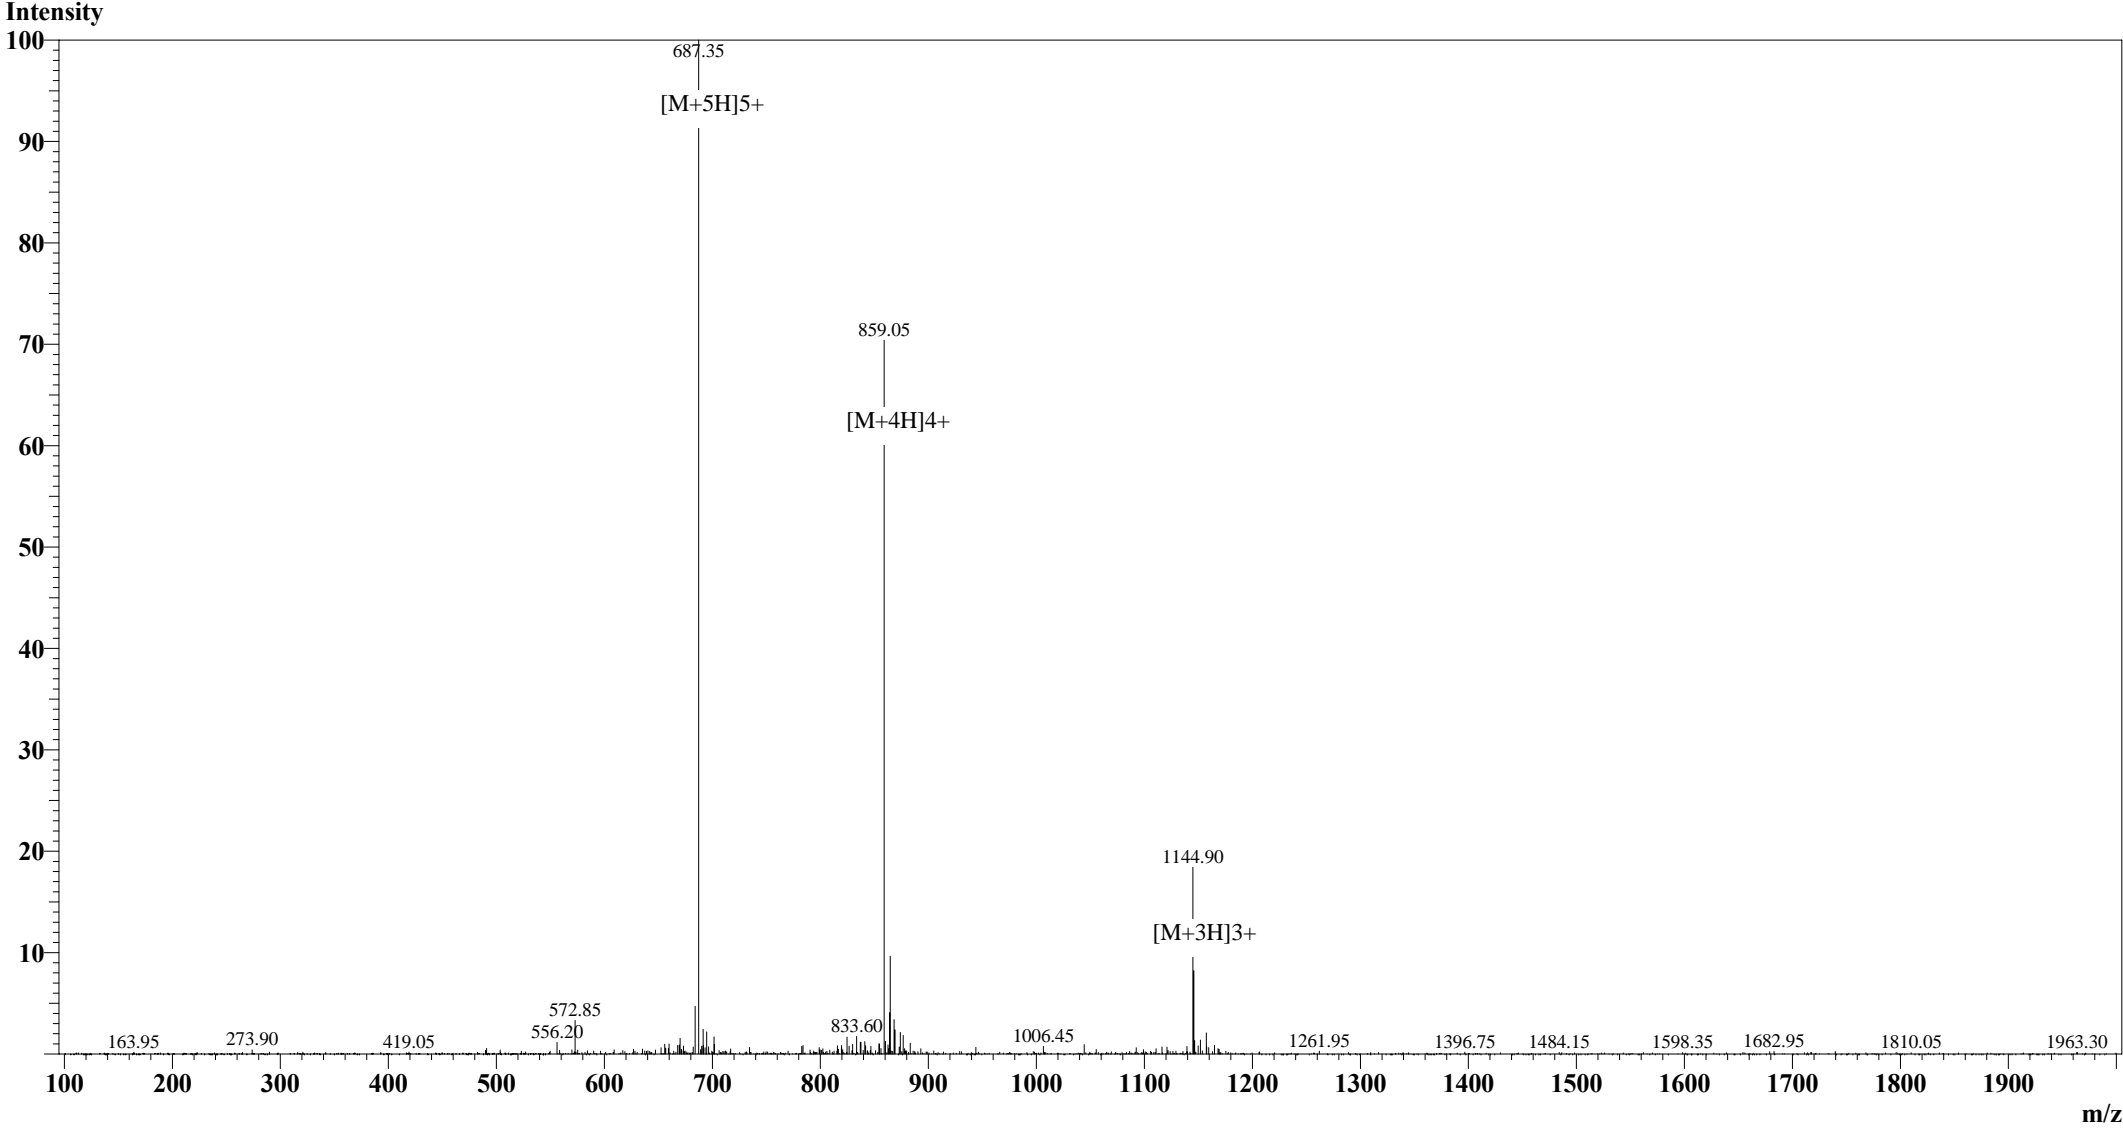

Sample Information		Interface		Prerod Bias	:+4.5kv
User	:Grace	Nebulizing Gas Flow	:1.50 L/min	Detector	:1.5kv
Date Acquired	: 06/03/2009 19:36:50	CDL Temp	: 250°C	T.Flow	: 0.2ml/min
Sample Name	:TLQP-30	CDL Volt	: -25.0V	B.conc	: 50%H2O/50%MeOH
Cat No.	: RP20245	Block Temp	: 200°C		
Lot No.	: CC01906				
Injection Volum	: 1.000µL				
Theoretical MW	: 3431.90				
Observed MW	: 3431.70				