

Sample Name : Aβ(18-28)
 Cat. No. : RP20105
 Lot. No. : CB03906


Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

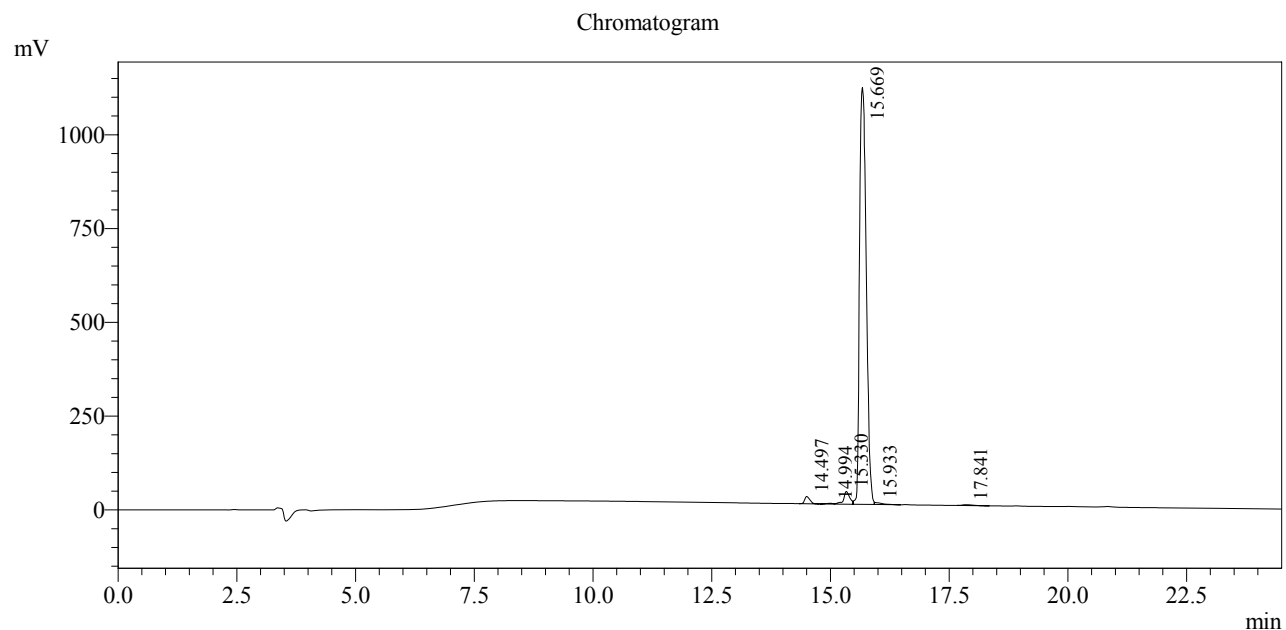

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	14.497	146978	19500	1.282
2	14.994	19913	1907	0.174
3	15.330	300493	34034	2.622
4	15.669	10897571	1111443	95.085
5	15.933	59271	5888	0.517
6	17.841	36663	2423	0.320
Total		11460889	1175195	100.000