

Sample Name : MbTP Ag85A
 Cat. No. : RP20202
 Lot. No. : CC07906

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
35.00	Pumps	Pump B Conc.	95	
35.01	Pumps	Pump B Conc.	5	
45.00	Pumps	Pump B Conc.	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

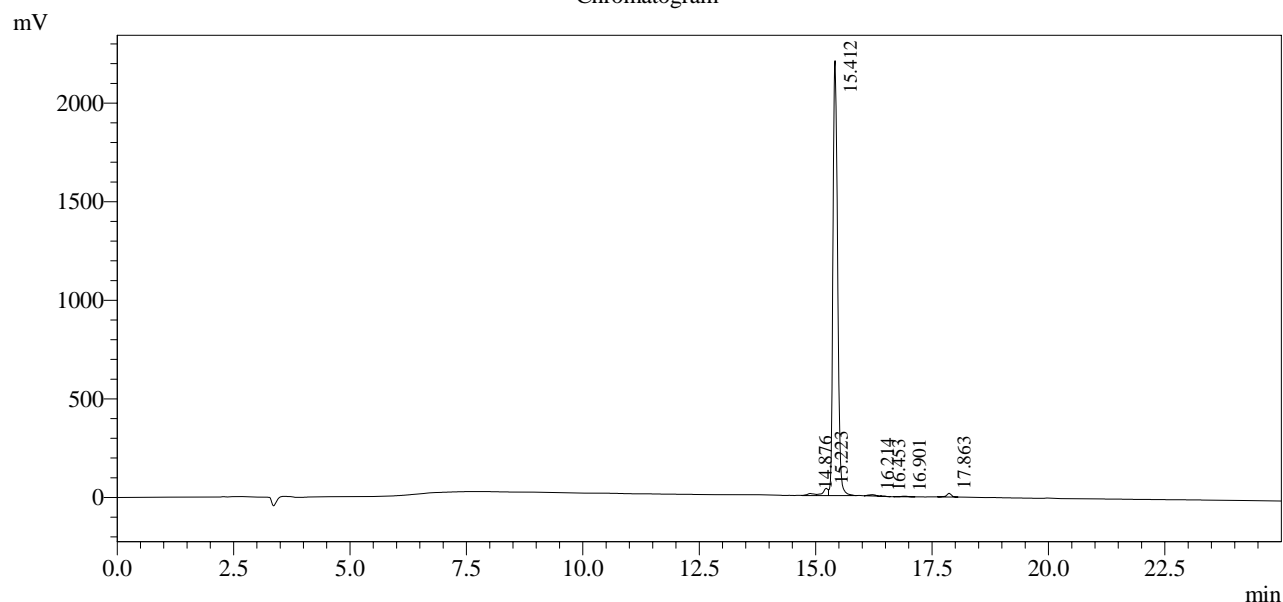

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	14.876	114196	10310	0.709
2	15.223	281861	36095	1.750
3	15.412	15453698	2205418	95.973
4	16.214	70429	6499	0.437
5	16.453	10041	1966	0.062
6	16.901	33777	3464	0.210
7	17.863	138198	18633	0.858
Total		16102200	2282385	100.000