

Sample Name : GRGDSP
 Cat. No. : RP20255
 Lot. No. : PE9651602

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

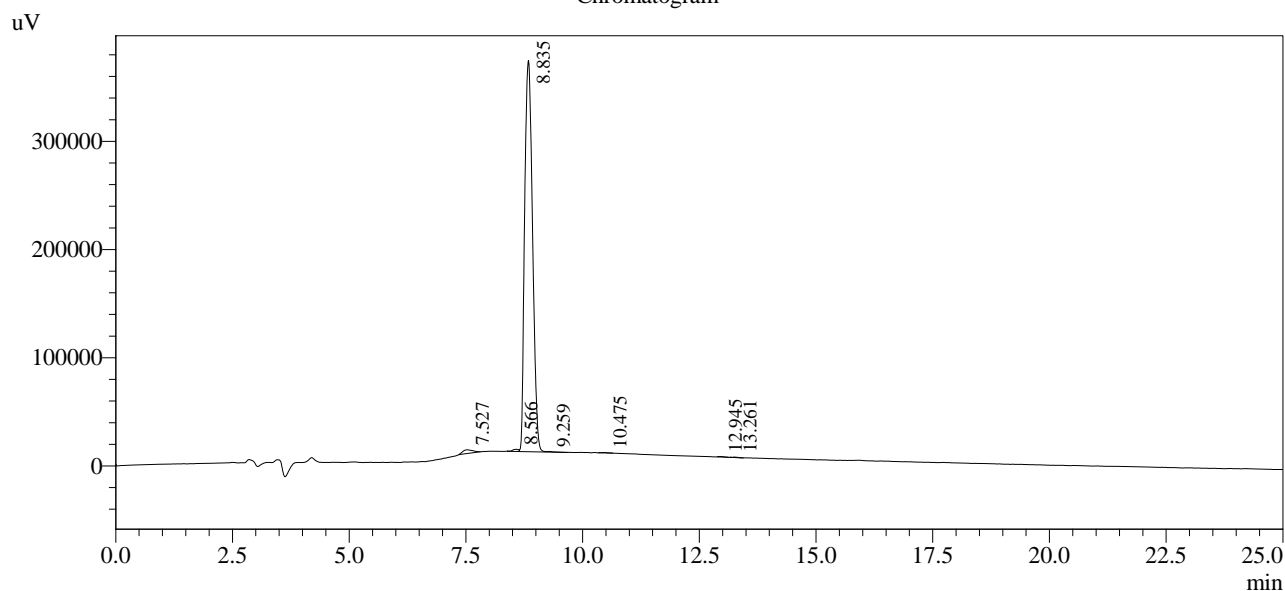

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.527	50786	3495	1.172
2	8.566	17259	1964	0.398
3	8.835	4249887	361518	98.056
4	9.259	7124	556	0.164
5	10.475	1878	368	0.043
6	12.945	3749	520	0.086
7	13.261	3465	383	0.080
Total		4334148	368804	100.000