

Sample Name :A-779
 Cat. No. :RP11249
 Lot. No. : PE9361605

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
45.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

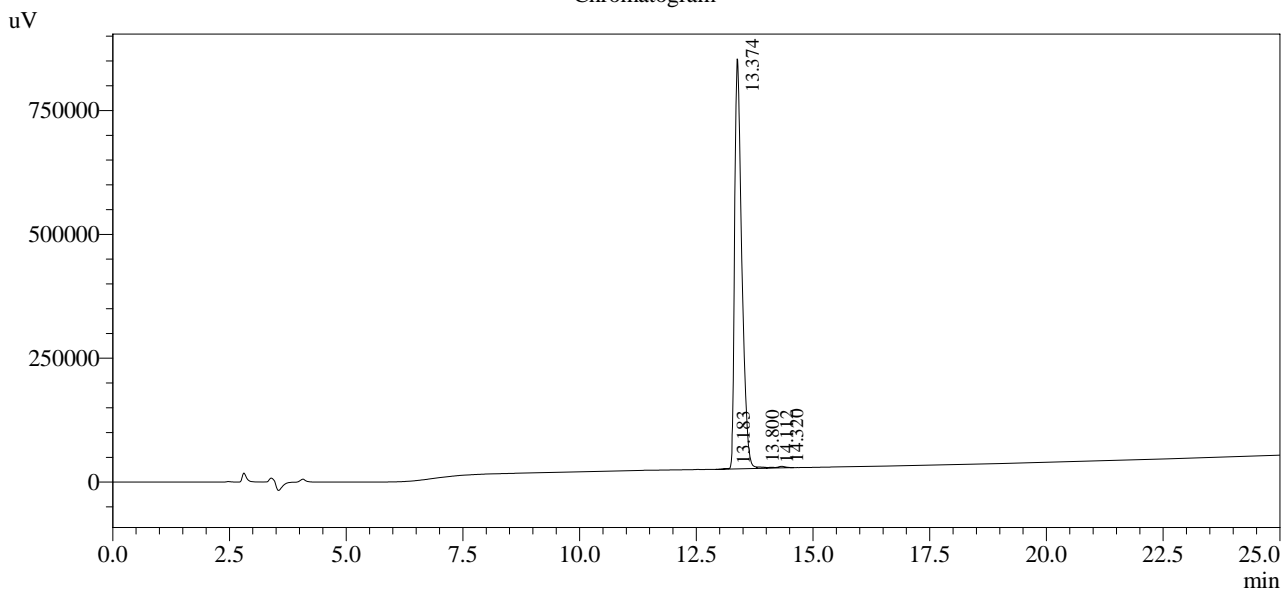

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.183	8373	1180	0.094
2	13.374	8832093	827763	98.954
3	13.800	31654	3001	0.355
4	14.112	17610	1722	0.197
5	14.320	35711	3203	0.400
Total		8925442	836870	100.000